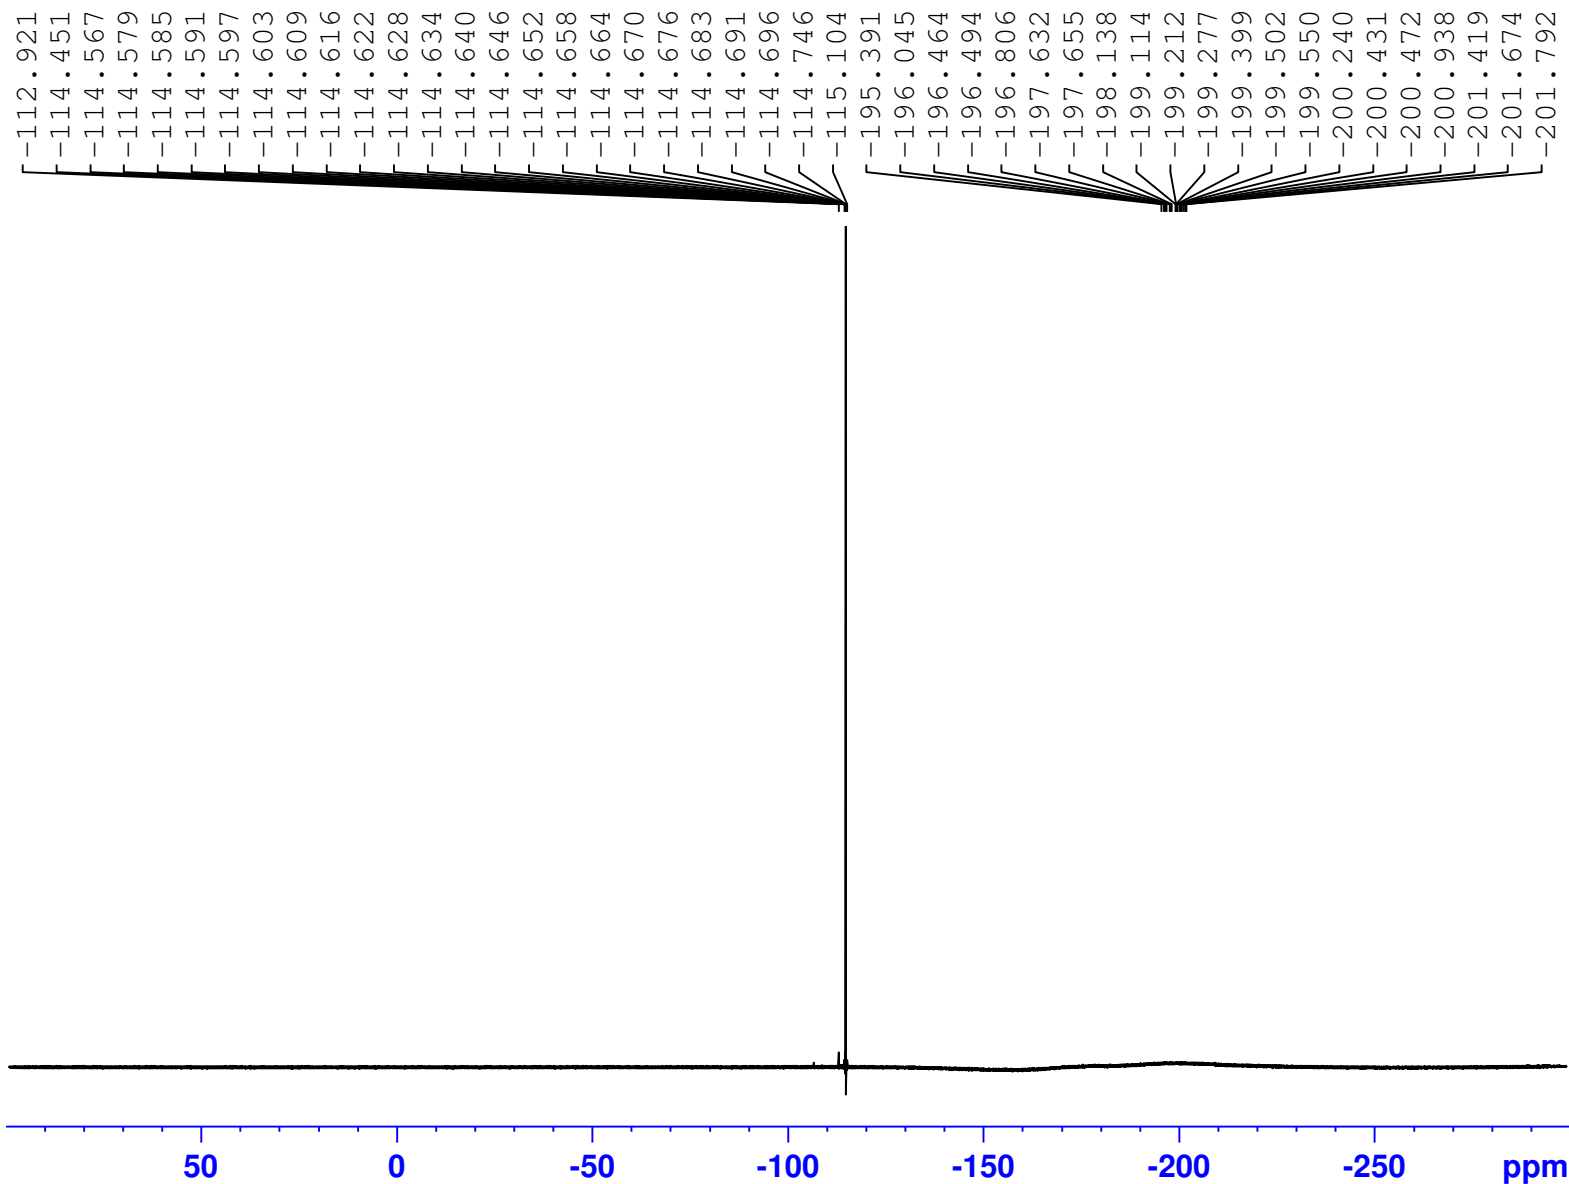


**Av400B**

Current Data Parameters  
 NAME Dec09-2019  
 EXPNO 22  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20191210  
 Time 0.09  
 INSTRUM spect  
 PROBHD 5 mm PABBO BB/  
 PULPROG zgfhigqn.2  
 TD 131072  
 SOLVENT MeOD  
 NS 16  
 DS 4  
 SWH 150000.000 Hz  
 FIDRES 1.144409 Hz  
 AQ 0.4369067 sec  
 RG 199.76  
 DW 3.333 usec  
 DE 6.50 usec  
 TE 298.0 K  
 D1 1.00000000 sec  
 D11 0.03000000 sec  
 D12 0.00002000 sec  
 TD0 1

===== CHANNEL f1 =====  
 SFO1 376.6394771 MHz  
 NUC1 19F  
 P1 11.00 usec  
 PLW1 32.00000000 W

===== CHANNEL f2 =====  
 SFO2 400.3216013 MHz  
 NUC2 1H  
 CPDPRG[2] waltz16  
 PCPD2 90.00 usec  
 PLW2 20.00000000 W  
 PLW12 0.29877001 W

F2 - Processing parameters  
 SI 131072  
 SF 376.6771450 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00