


Av400B

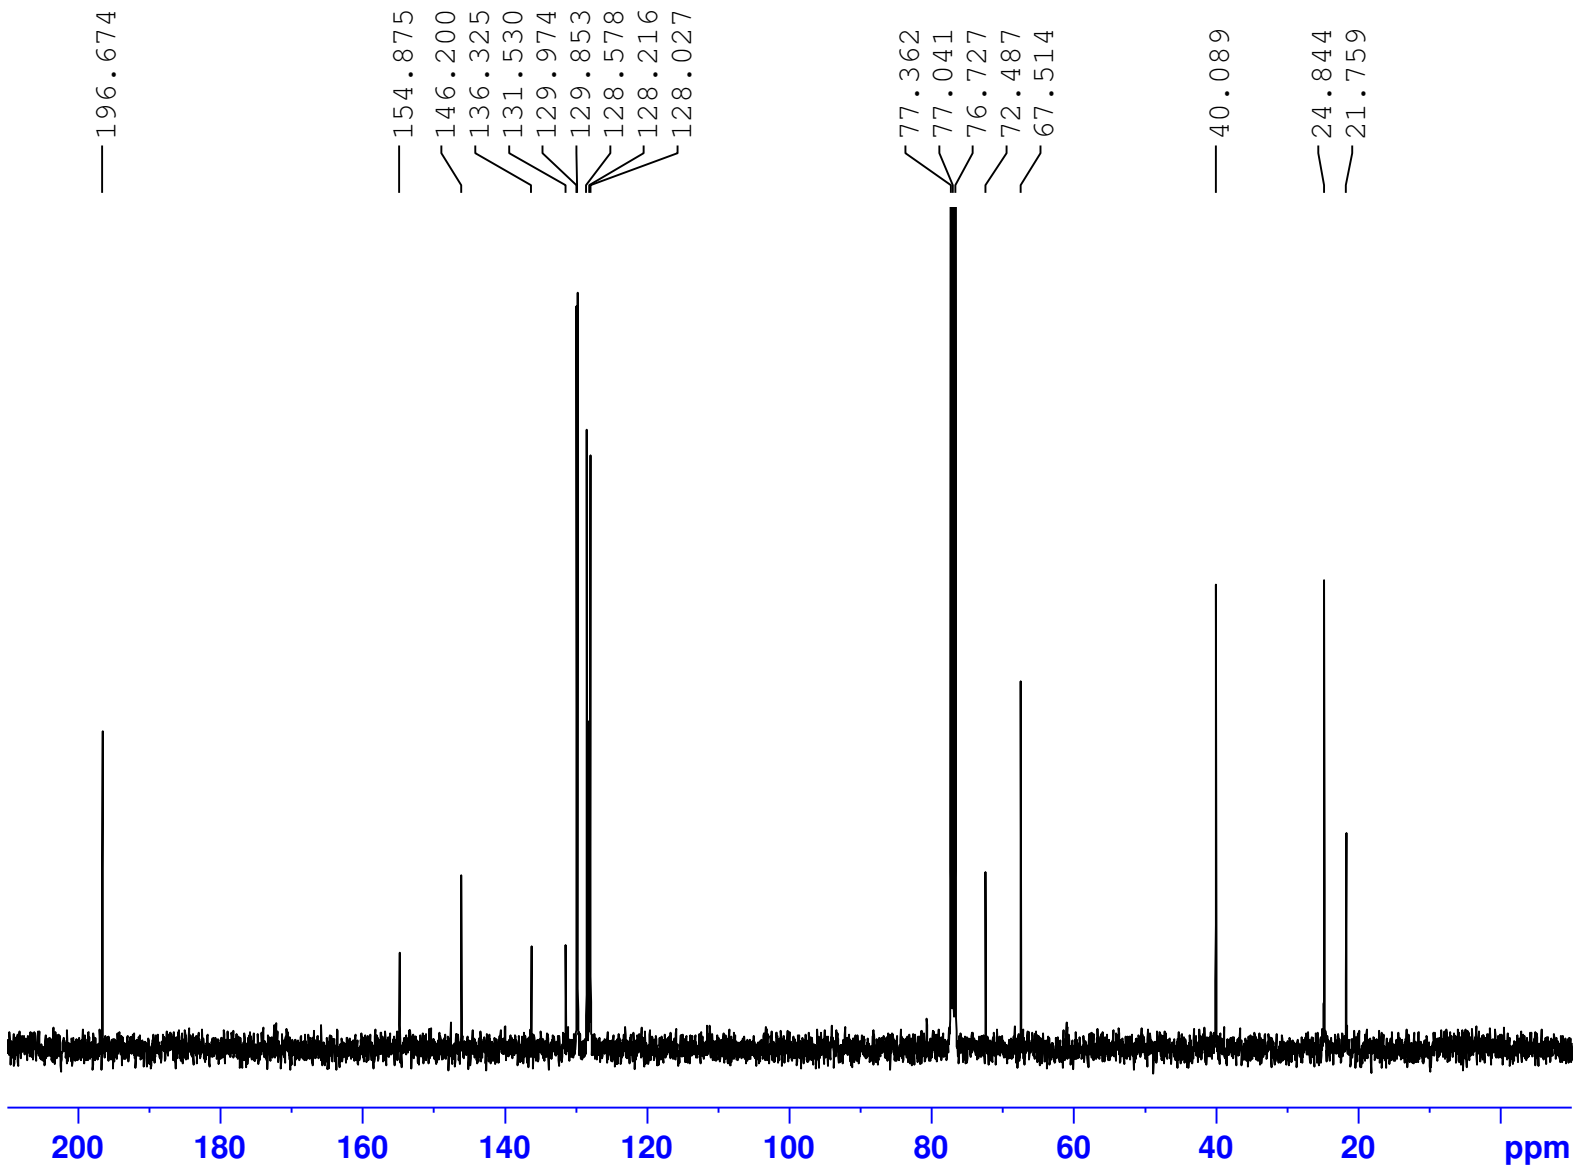

Current Data Parameters	
NAME	Sep18-2019
EXPNO	90
PROCNO	1

```

F2 - Acquisition Parameters
Date_      20190918
Time       18.17
INSTRUM    spect
PROBHD     5 mm PABBO BB/
PULPROG    zgpg30
TD          32768
SOLVENT    CDC13
NS          352
DS          4
SWH         28409.092 Hz
FIDRES     0.866977 Hz
AQ          0.5767168 sec
RG          199.76
DW          17.600 used
DE          6.50 used
TE          295.4 K
D1          1.00000000 sec
D11         0.03000000 sec
TD0         1

```

```
===== CHANNEL f1 =====
SFO1      100.6716167 MHz
NUC1              13C
P1              9.80 usec
PLW1      50.11899948 W
```

```
===== CHANNEL f2 =====
SFO2          400.3220016 MHz
NUC2          1H
CPDPRG[2]     waltz16
PCPD2         90.00 usec
PLW2          20.00000000 W
PLW12         0.29877001 W
PLW13         0.24200000 W
```

F2 - Processing parameters	
SI	16384
SF	100.6605440 MHz
WDW	EM
SSB	0
LB	2.00 Hz
GB	0
PC	1.20