


# Av-400C

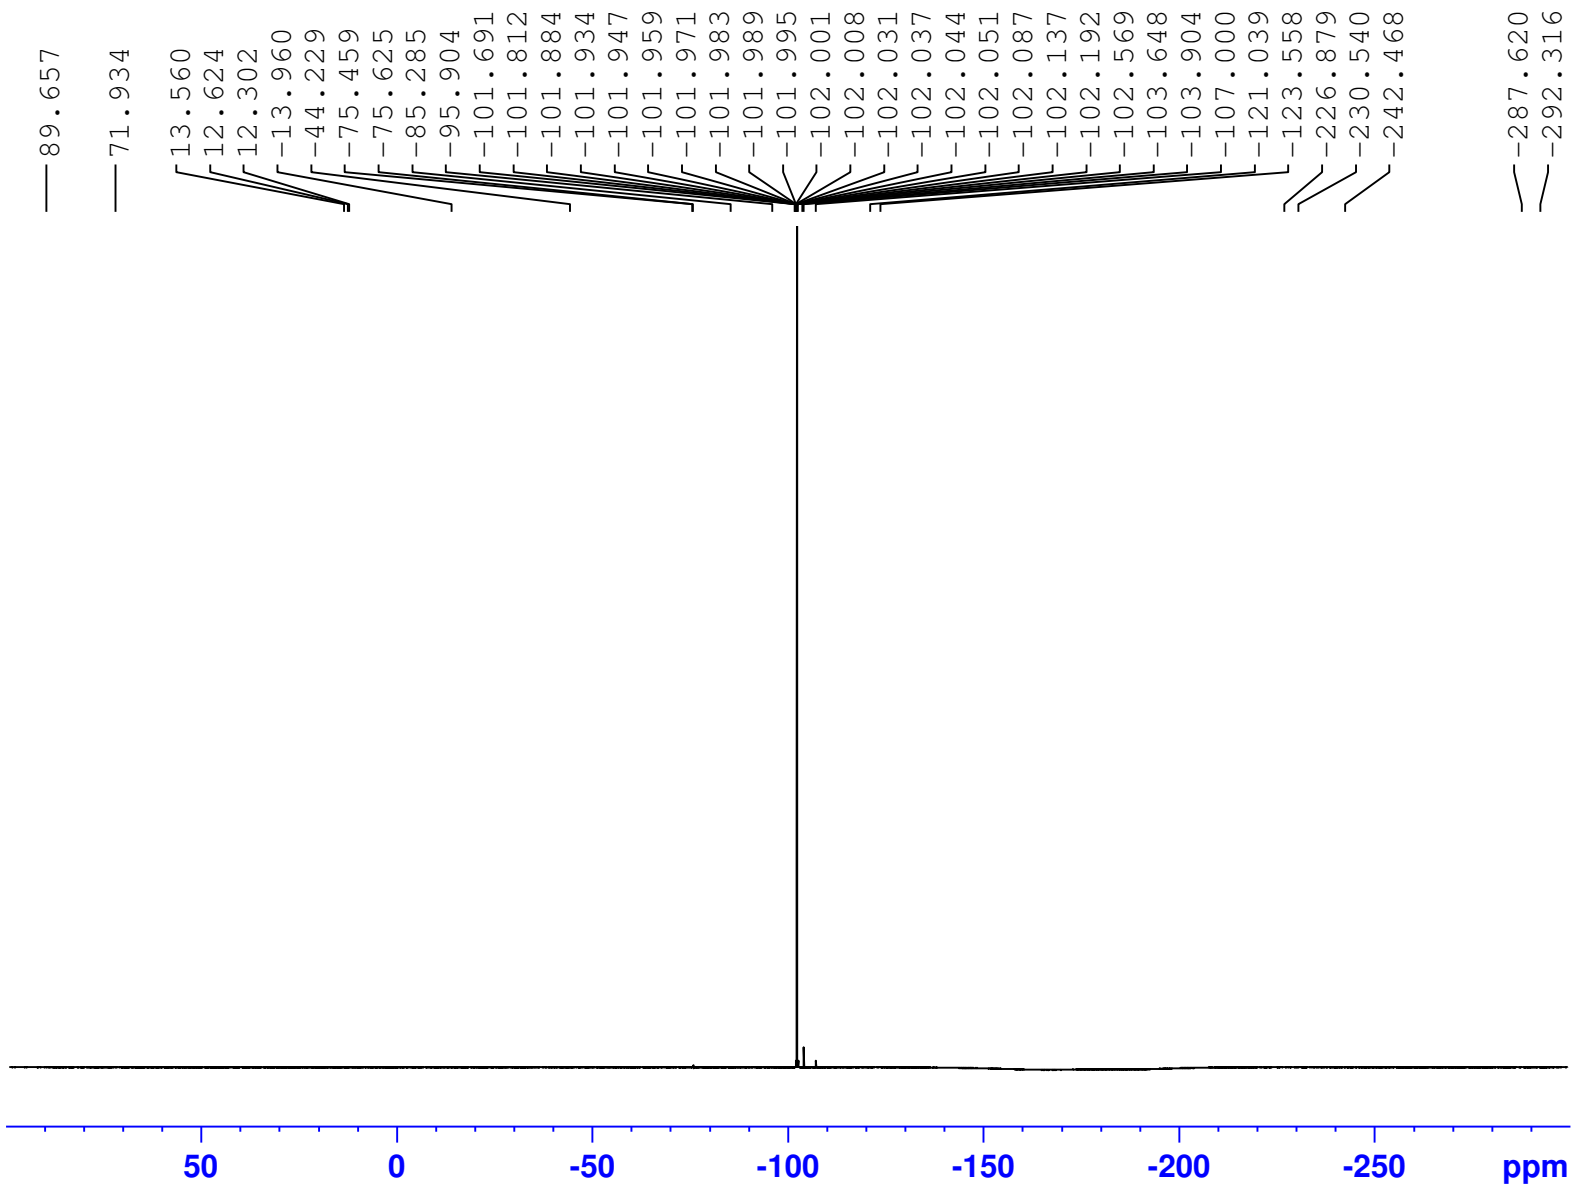

-287.620  
-292.316

Current Data Parameters  
 NAME Nov07-2019  
 EXPNO 52  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20191108  
 Time 0.27  
 INSTRUM spect  
 PROBHD 5 mm PABBO BB/  
 PULPROG zgfhigqn.2  
 TD 131072  
 SOLVENT CDC13  
 NS 16  
 DS 4  
 SWH 150000.000 Hz  
 FIDRES 1.144409 Hz  
 AQ 0.4369067 sec  
 RG 199.33  
 DW 3.333 usec  
 DE 6.50 usec  
 TE 294.8 K  
 D1 1.00000000 sec  
 D11 0.03000000 sec  
 D12 0.00002000 sec  
 TD0 1

===== CHANNEL f1 =====  
 SFO1 376.5265756 MHz  
 NUC1 19F  
 P1 12.00 usec  
 PLW1 25.11899948 W

===== CHANNEL f2 =====  
 SFO2 400.2016008 MHz  
 NUC2 1H  
 CPDPRG[2] waltz16  
 PCPD2 90.00 usec  
 PLW2 19.95299911 W  
 PLW12 0.33147001 W

F2 - Processing parameters  
 SI 131072  
 SF 376.5642320 MHz  
 WDW EM  
 SSB 0  
 LB 3.00 Hz  
 GB 0  
 PC 1.00