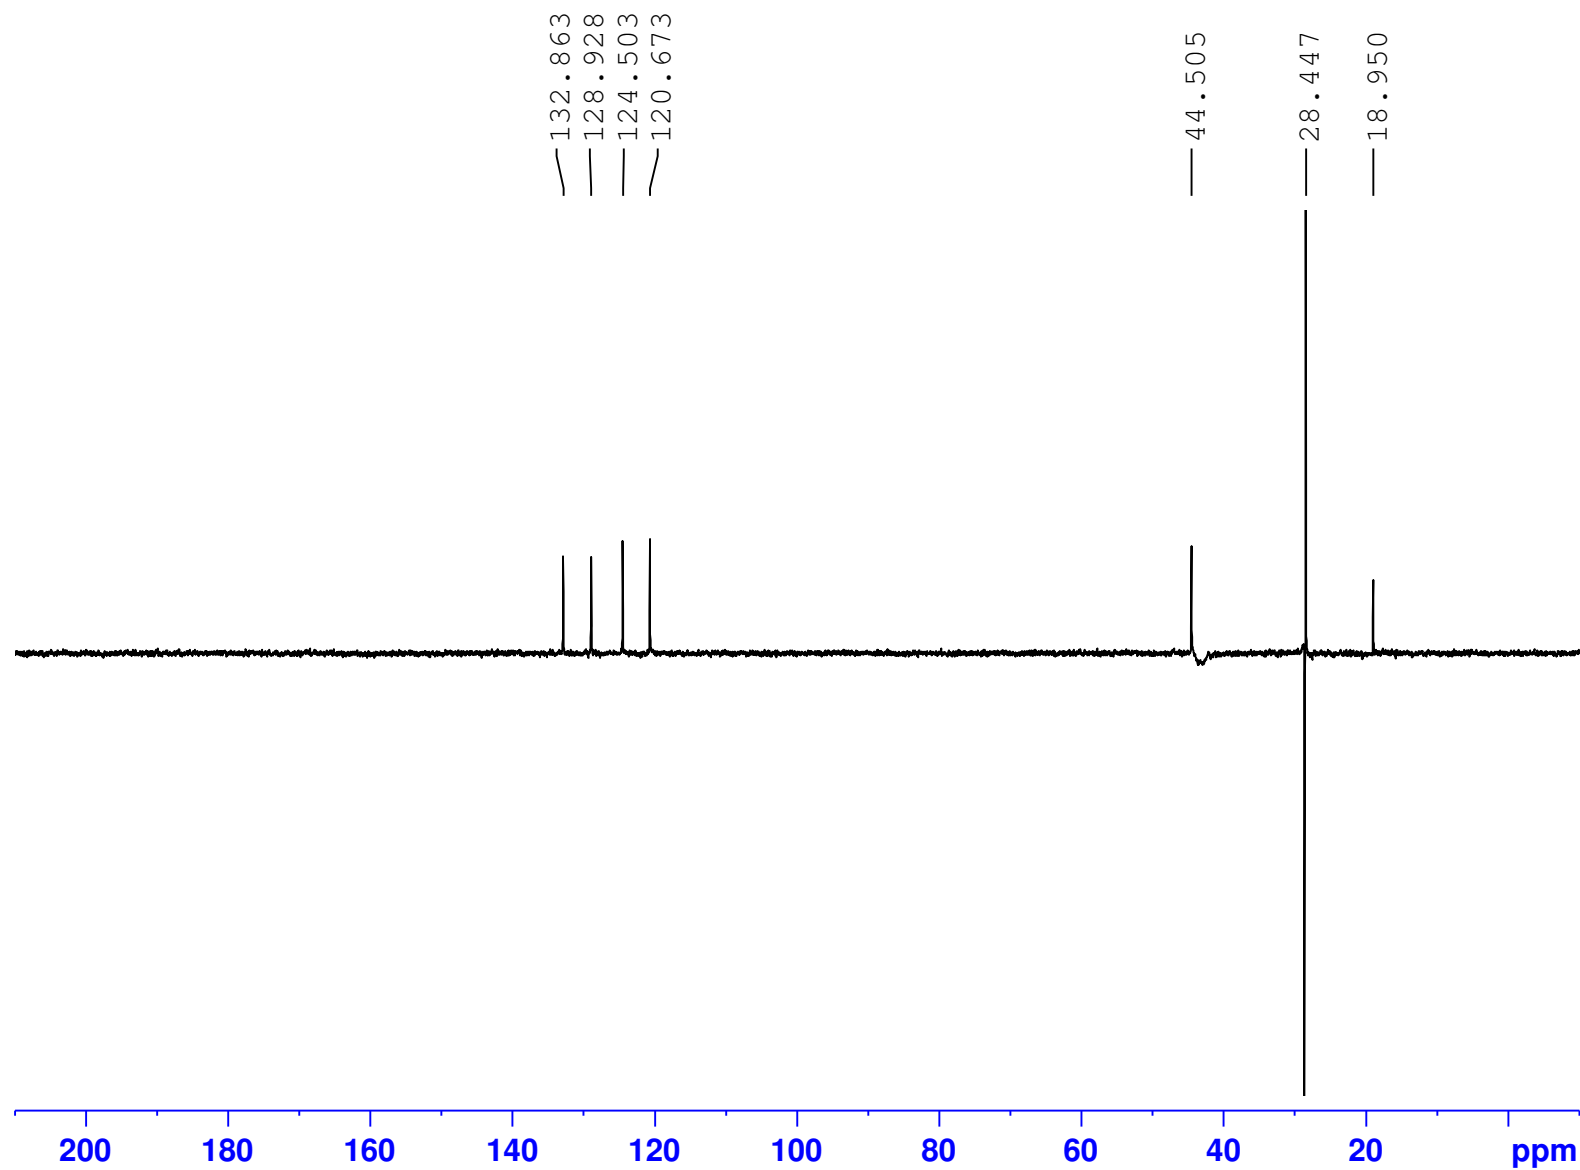


Av-500

Current Data Parameters
NAME Feb19-2021
EXPNO 153
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210220
Time 13.41
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG dept135
TD 32768
SOLVENT CDCl3
NS 386
DS 4
SWH 26315.789 Hz
FIDRES 0.803094 Hz
AQ 0.6225920 sec
RG 207.33
DW 19.000 usec
DE 6.50 usec
TE 294.6 K
CNST2 145.0000000
D1 1.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 100.6942493 MHz
NUC1 ^{13}C
P1 9.60 usec
P2 19.20 usec
PLW1 59.97900009 W

===== CHANNEL f2 =====
SFO2 400.4119220 MHz
NUC2 ^1H
CPDPRG[2] waltz16
P3 11.25 usec
P4 22.50 usec
PCPD2 90.00 usec
PLW2 19.95299911 W
PLW12 0.31176999 W

F2 - Processing parameters
SI 16384
SF 100.6831750 MHz
WDW EM
SSB 0
LB 2.50 Hz
GB 0
PC 1.40