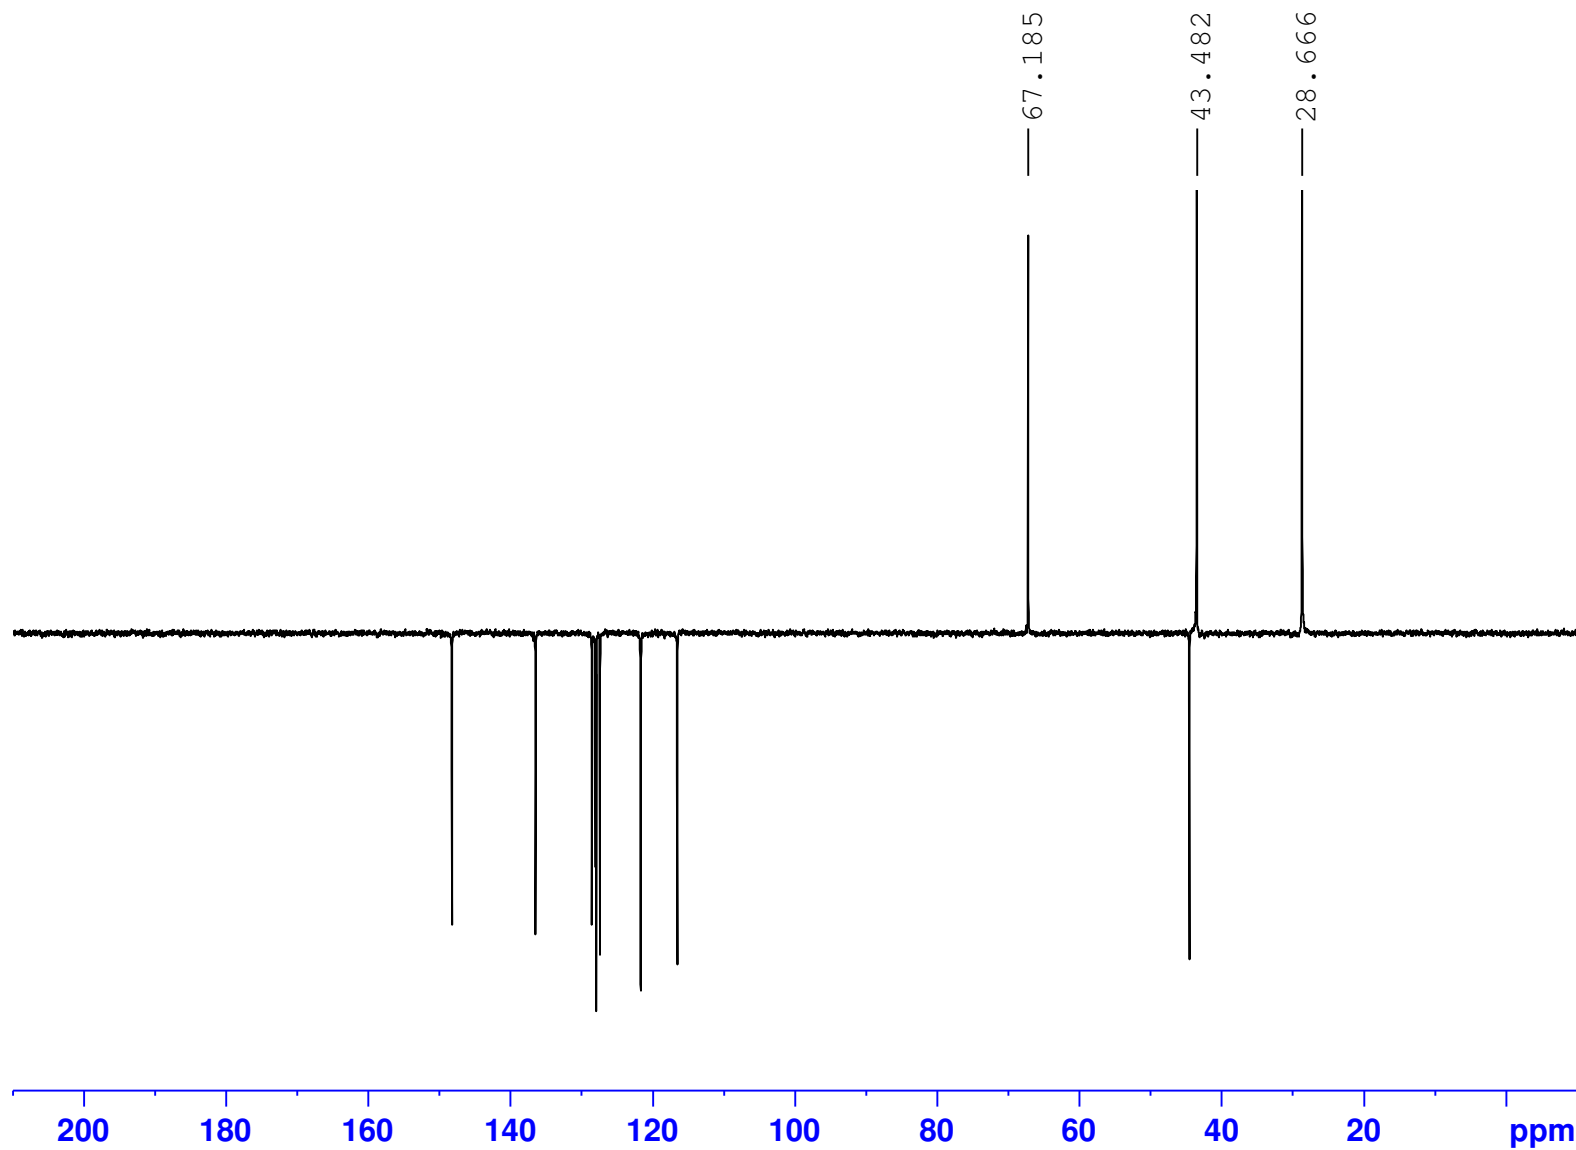


**Av-500**

Current Data Parameters  
NAME Feb19-2021  
EXPNO 163  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20210220  
Time 14.40  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG dept135  
TD 32768  
SOLVENT CDCl3  
NS 386  
DS 4  
SWH 26315.789 Hz  
FIDRES 0.803094 Hz  
AQ 0.6225920 sec  
RG 207.33  
DW 19.000 usec  
DE 6.50 usec  
TE 294.6 K  
CNST2 145.0000000  
D1 1.00000000 sec  
D2 0.00344828 sec  
D12 0.00002000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 100.6942493 MHz  
NUC1 13C  
P1 9.60 usec  
P2 19.20 usec  
PLW1 59.97900009 W

===== CHANNEL f2 =====  
SFO2 400.4119220 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
P3 11.25 usec  
P4 22.50 usec  
PCPD2 90.00 usec  
PLW2 19.95299911 W  
PLW12 0.31176999 W

F2 - Processing parameters  
SI 16384  
SF 100.6831750 MHz  
WDW EM  
SSB 0  
LB 2.50 Hz  
GB 0  
PC 1.40