


SP266B

Av400B

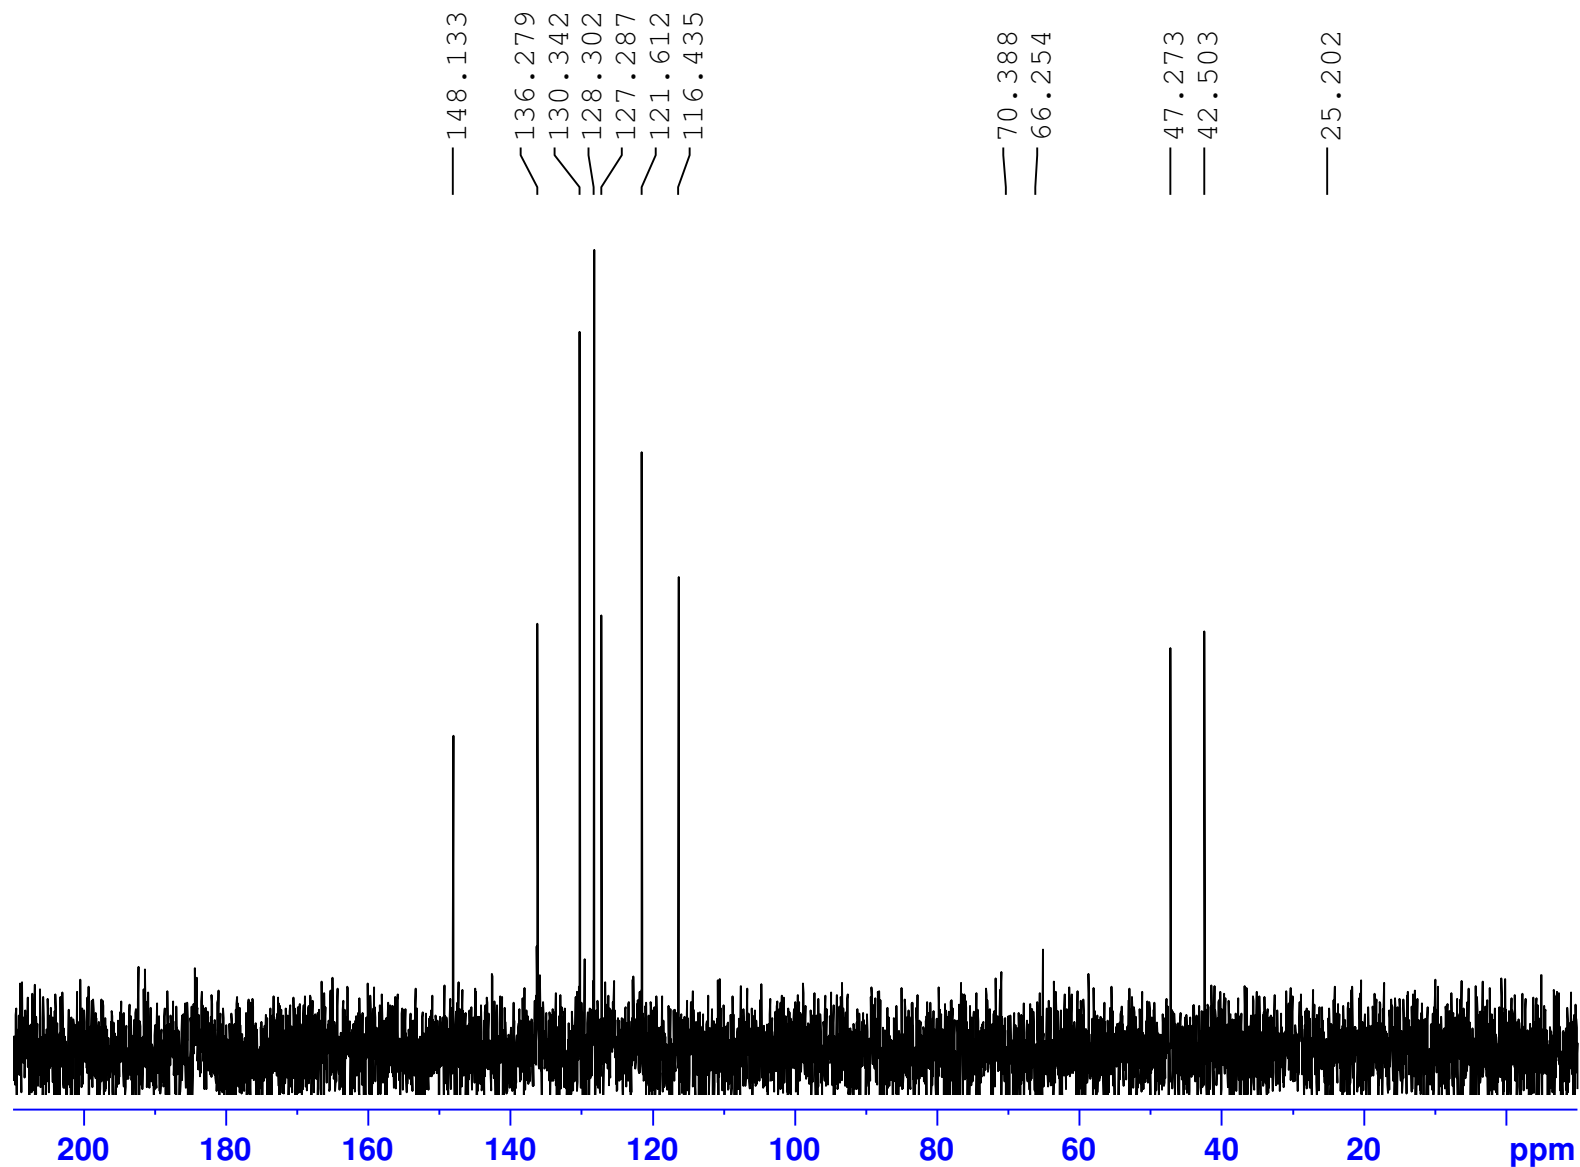

Current Data Parameters
NAME Feb19-2021
EXPNO 22
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210220
Time 13.52
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG dept135
TD 32768
SOLVENT CDCl3
NS 344
DS 4
SWH 28409.092 Hz
FIDRES 0.866977 Hz
AQ 0.5767168 sec
RG 199.76
DW 17.600 usec
DE 6.50 usec
TE 295.2 K
CNST2 145.0000000
D1 1.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 100.6716167 MHz
NUC1 13C
P1 9.80 usec
P2 19.60 usec
PLW1 50.11899948 W

===== CHANNEL f2 =====
SFO2 400.3220016 MHz
NUC2 1H
CPDPRG[2] waltz16
P3 11.00 usec
P4 22.00 usec
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.29877001 W

F2 - Processing parameters
SI 16384
SF 100.6605440 MHz
WDW EM
SSB 0
LB 2.00 Hz
GB 0
PC 1.40