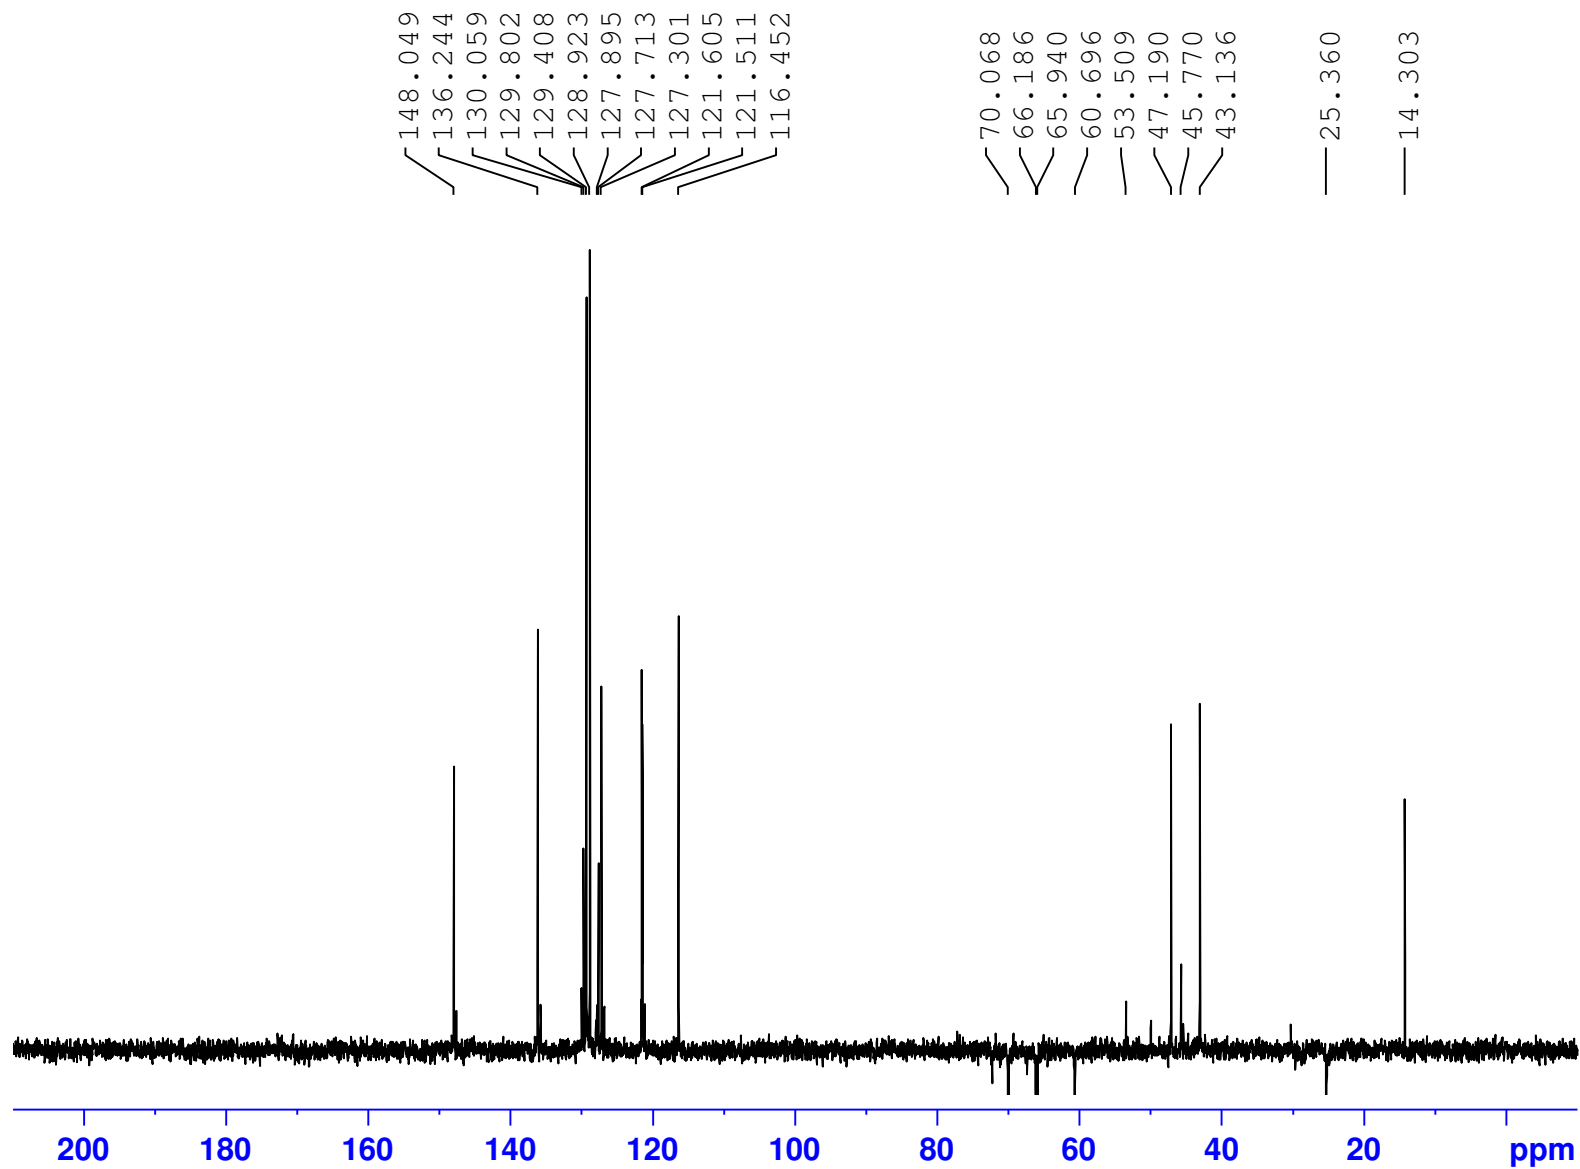


**Av400B**

Current Data Parameters  
NAME Feb19-2021  
EXPNO 42  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20210220  
Time 16.10  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG dept135  
TD 32768  
SOLVENT CDCl3  
NS 344  
DS 4  
SWH 28409.092 Hz  
FIDRES 0.866977 Hz  
AQ 0.5767168 sec  
RG 199.76  
DW 17.600 usec  
DE 6.50 usec  
TE 295.2 K  
CNST2 145.0000000  
D1 1.00000000 sec  
D2 0.00344828 sec  
D12 0.00002000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 100.6716167 MHz  
NUC1 13C  
P1 9.80 usec  
P2 19.60 usec  
PLW1 50.11899948 W

===== CHANNEL f2 =====  
SFO2 400.3220016 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
P3 11.00 usec  
P4 22.00 usec  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.29877001 W

F2 - Processing parameters  
SI 16384  
SF 100.6605440 MHz  
WDW EM  
SSB 0  
LB 2.00 Hz  
GB 0  
PC 1.40