


NMR System BNMR_311-1 400 BH013110
Pfizer Confidential
carbon CDCl3 {C:\Bruker\TopSpin3.0} duboim06 32

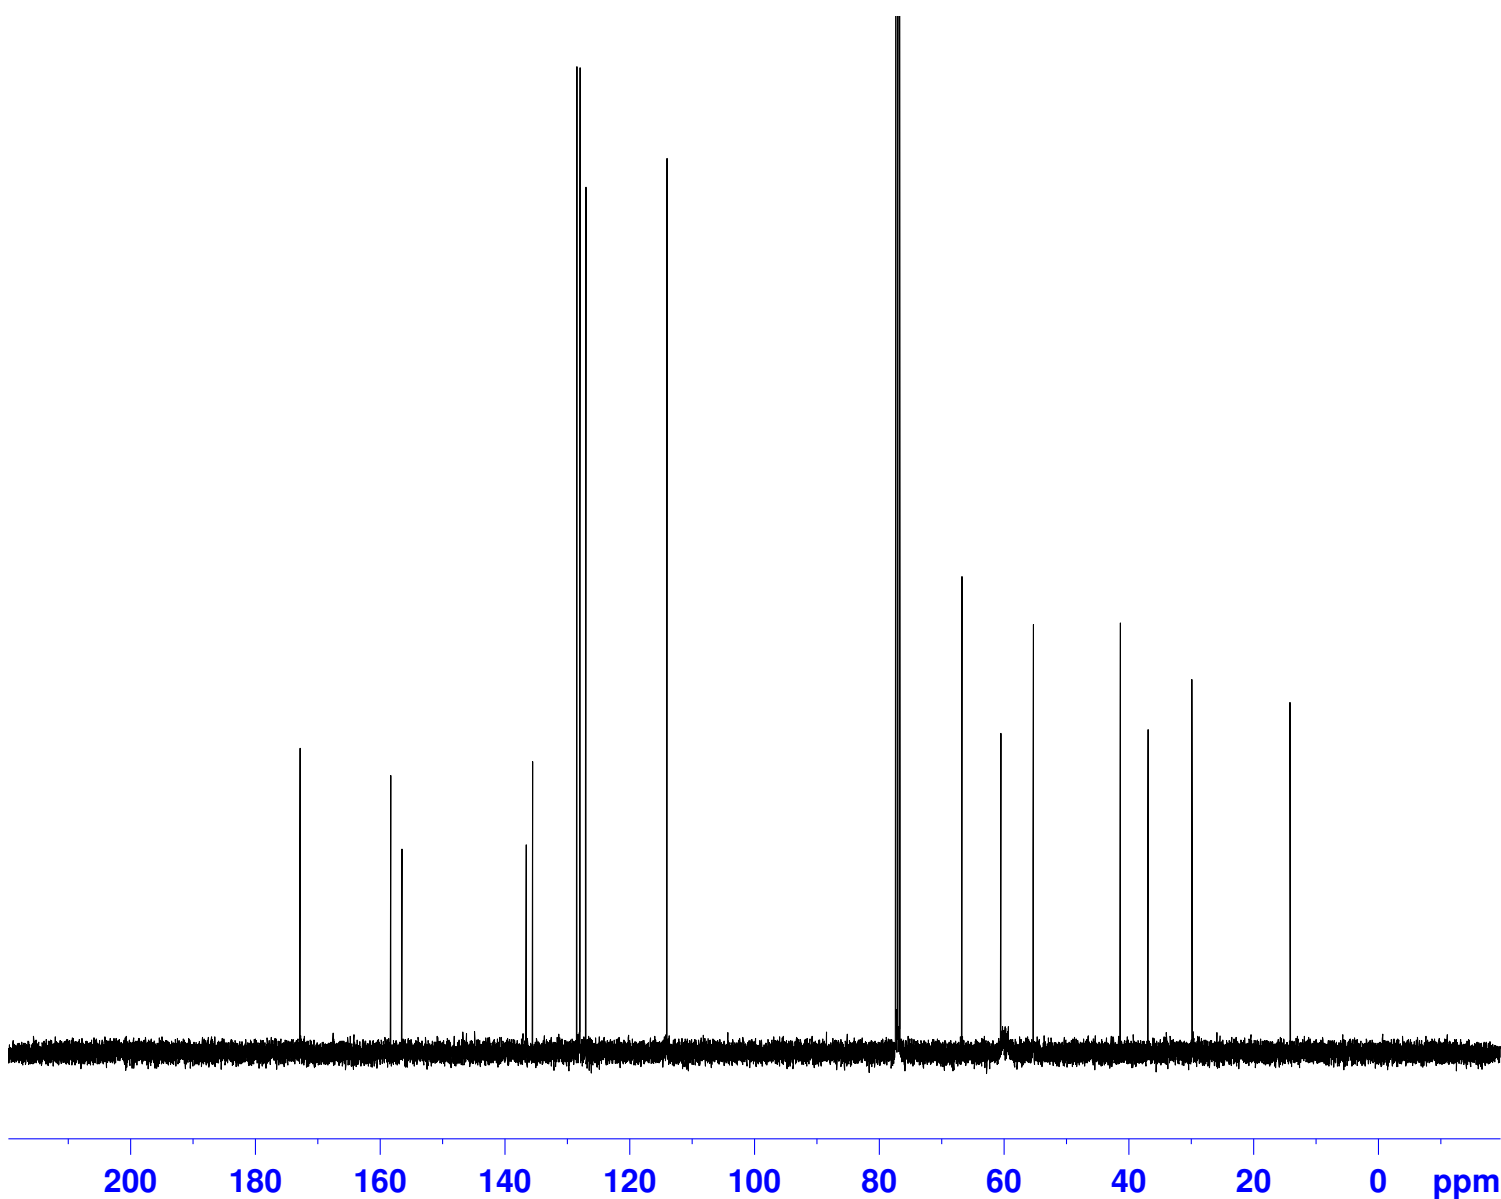

Current Data Parameters
NAME 00712940-0087-C
EXPNO 2
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180809
Time 10.16
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zgpg30
TD 65536
SOLVENT CDCl3
NS 512
DS 4
SWH 24038.461 Hz
FIDRES 0.366798 Hz
AQ 1.3631488 sec
RG 193.07
DW 20.800 usec
DE 6.50 usec
TE 300.1 K
D1 0.89999998 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 100.5197265 MHz
NUC1 13C
P1 8.00 usec
PLW1 80.00000000 W

===== CHANNEL f2 =====
SFO2 399.7215992 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 29.99200058 W
PLW12 0.34123999 W
PLW13 0.27640000 W

F2 - Processing parameters
SI 65536
SF 100.5096740 MHz
WDW EM
SSB 0
LB 0.39 Hz
GB 0
PC 1.40