


Diethylzinc

Av-400C

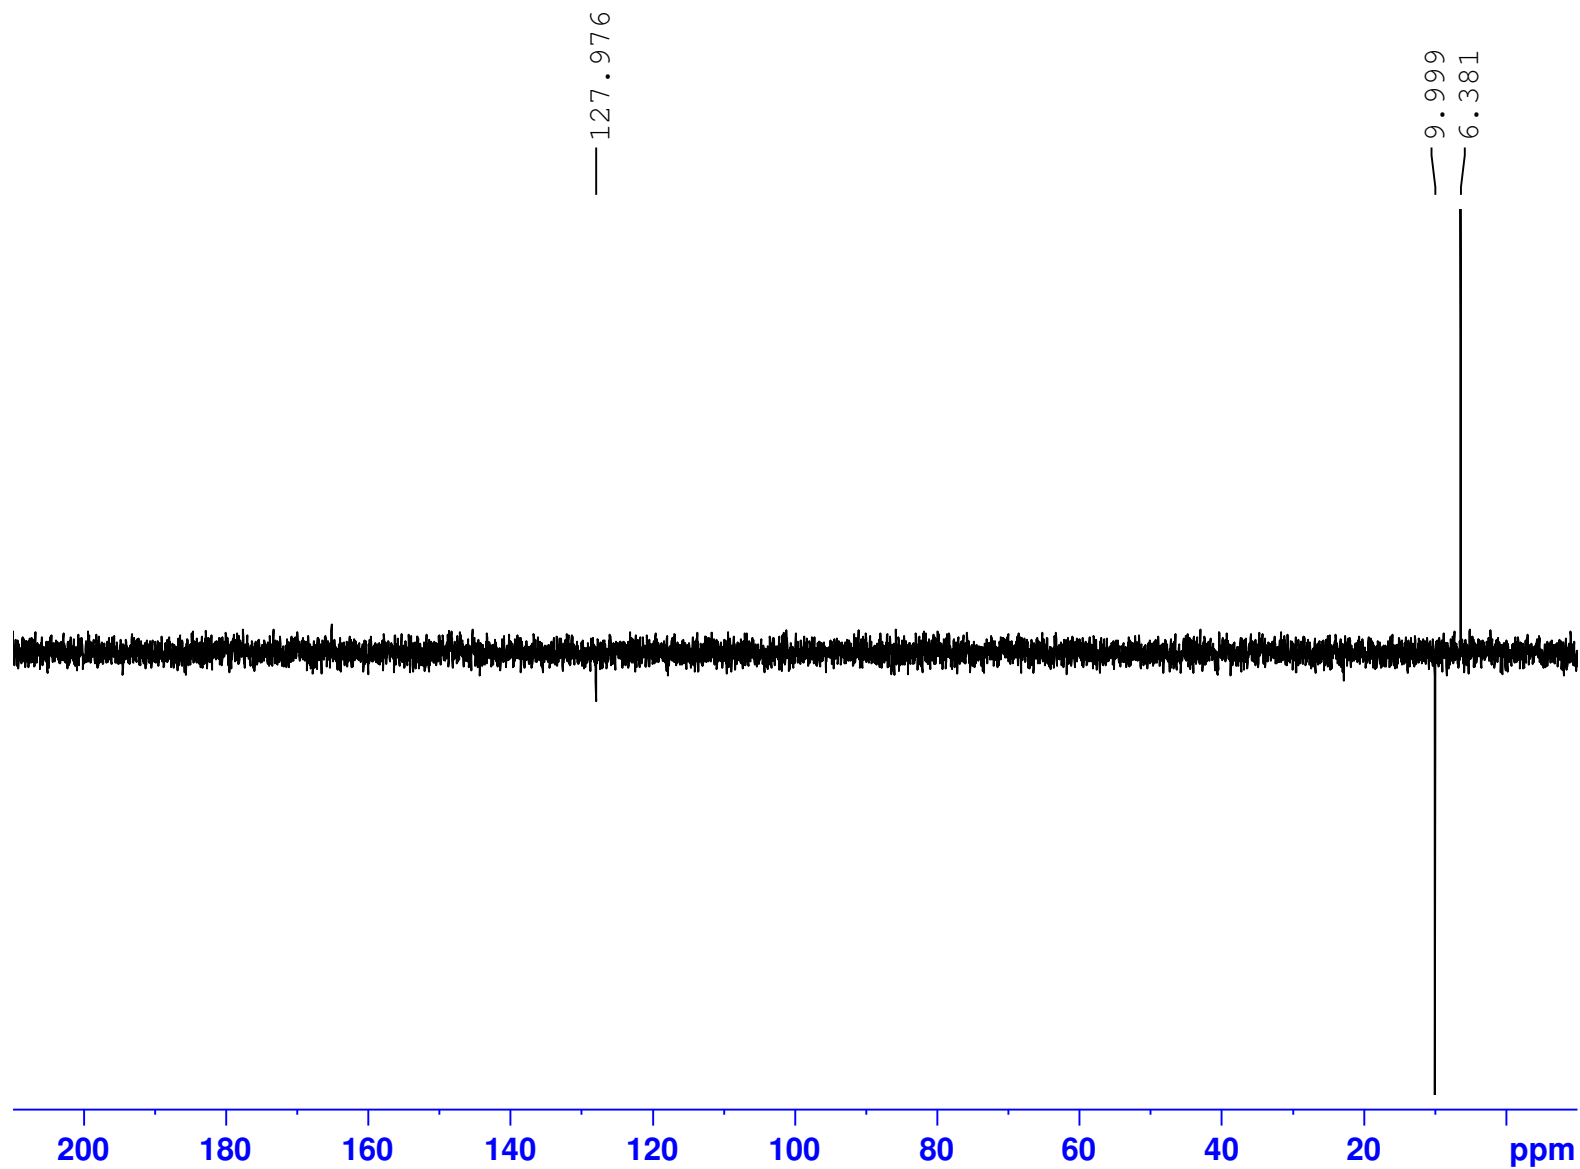

Current Data Parameters
NAME Jun24-2016
EXPNO 12
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160625
Time 4.01
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG dept135
TD 32768
SOLVENT C6D6
NS 360
DS 4
SWH 28409.092 Hz
FIDRES 0.866977 Hz
AQ 0.5767168 sec
RG 199.33
DW 17.600 usec
DE 6.50 usec
TE 297.7 K
CNST2 145.000000
D1 1.00000000 sec
D2 0.00344828 sec
D12 0.00002000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 100.6414394 MHz
NUC1 13C
P1 9.50 usec
P2 19.00 usec
PLW1 60.25600052 W

===== CHANNEL f2 =====
SFO2 400.2020010 MHz
NUC2 1H
CPDPRG[2] waltz16
P3 10.50 usec
P4 21.00 usec
PCPD2 90.00 usec
PLW2 19.95299911 W
PLW12 0.27158001 W

F2 - Processing parameters
SI 16384
SF 100.6303700 MHz
WDW EM
SSB 0
LB 2.00 Hz
GB 0
PC 1.40