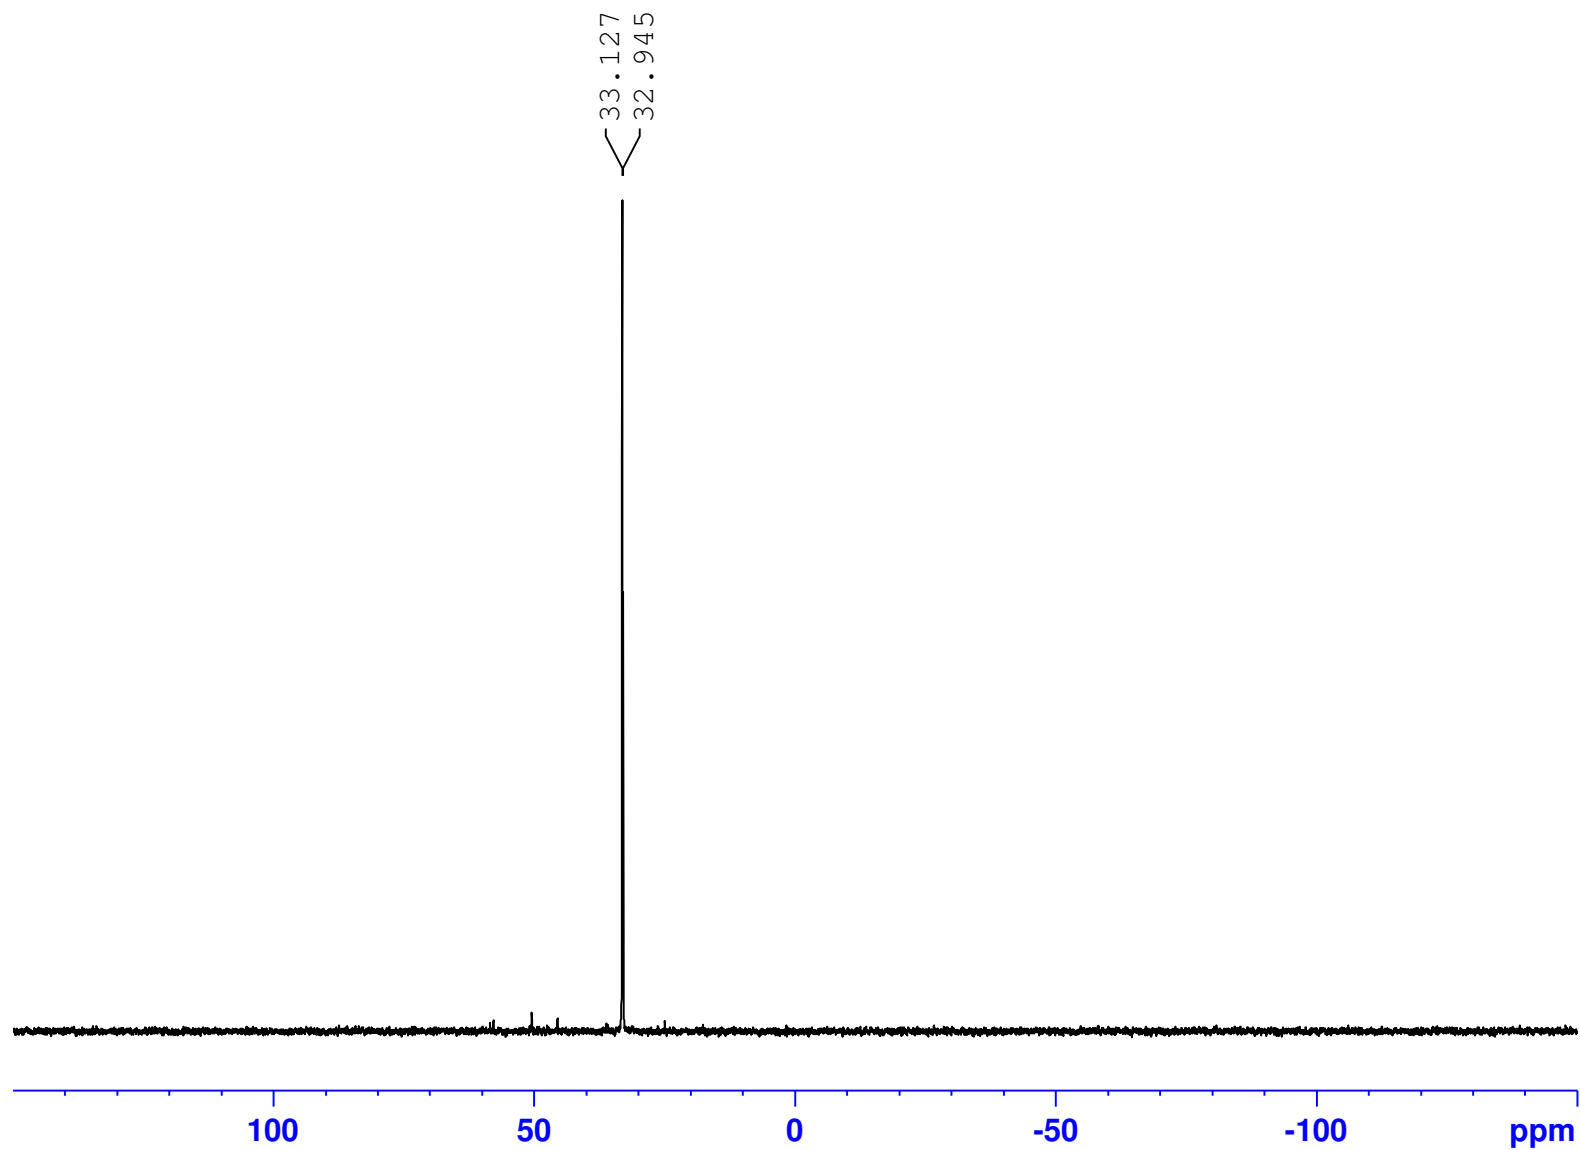


Av-400A

Current Data Parameters
NAME Marl7-2020
EXPNO 215
PROCNO 1

F2 - Acquisition Parameters
Date_ 20200317
Time 14.45
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zgpg30
TD 32768
SOLVENT CDCl3
NS 60
DS 4
SWH 64102.562 Hz
FIDRES 1.956255 Hz
AQ 0.2555904 sec
RG 207.33
DW 7.800 usec
DE 6.50 usec
TE 294.6 K
D1 2.50000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 162.0873182 MHz
NUC1 31P
P1 6.20 usec
PLW1 59.97900009 W

===== CHANNEL f2 =====
SFO2 400.4119220 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 19.95299911 W
PLW12 0.19953001 W
PLW13 0.16162001 W

F2 - Processing parameters
SI 32768
SF 162.0889390 MHz
WDW EM
SSB 0
LB 4.00 Hz
GB 0
PC 1.40