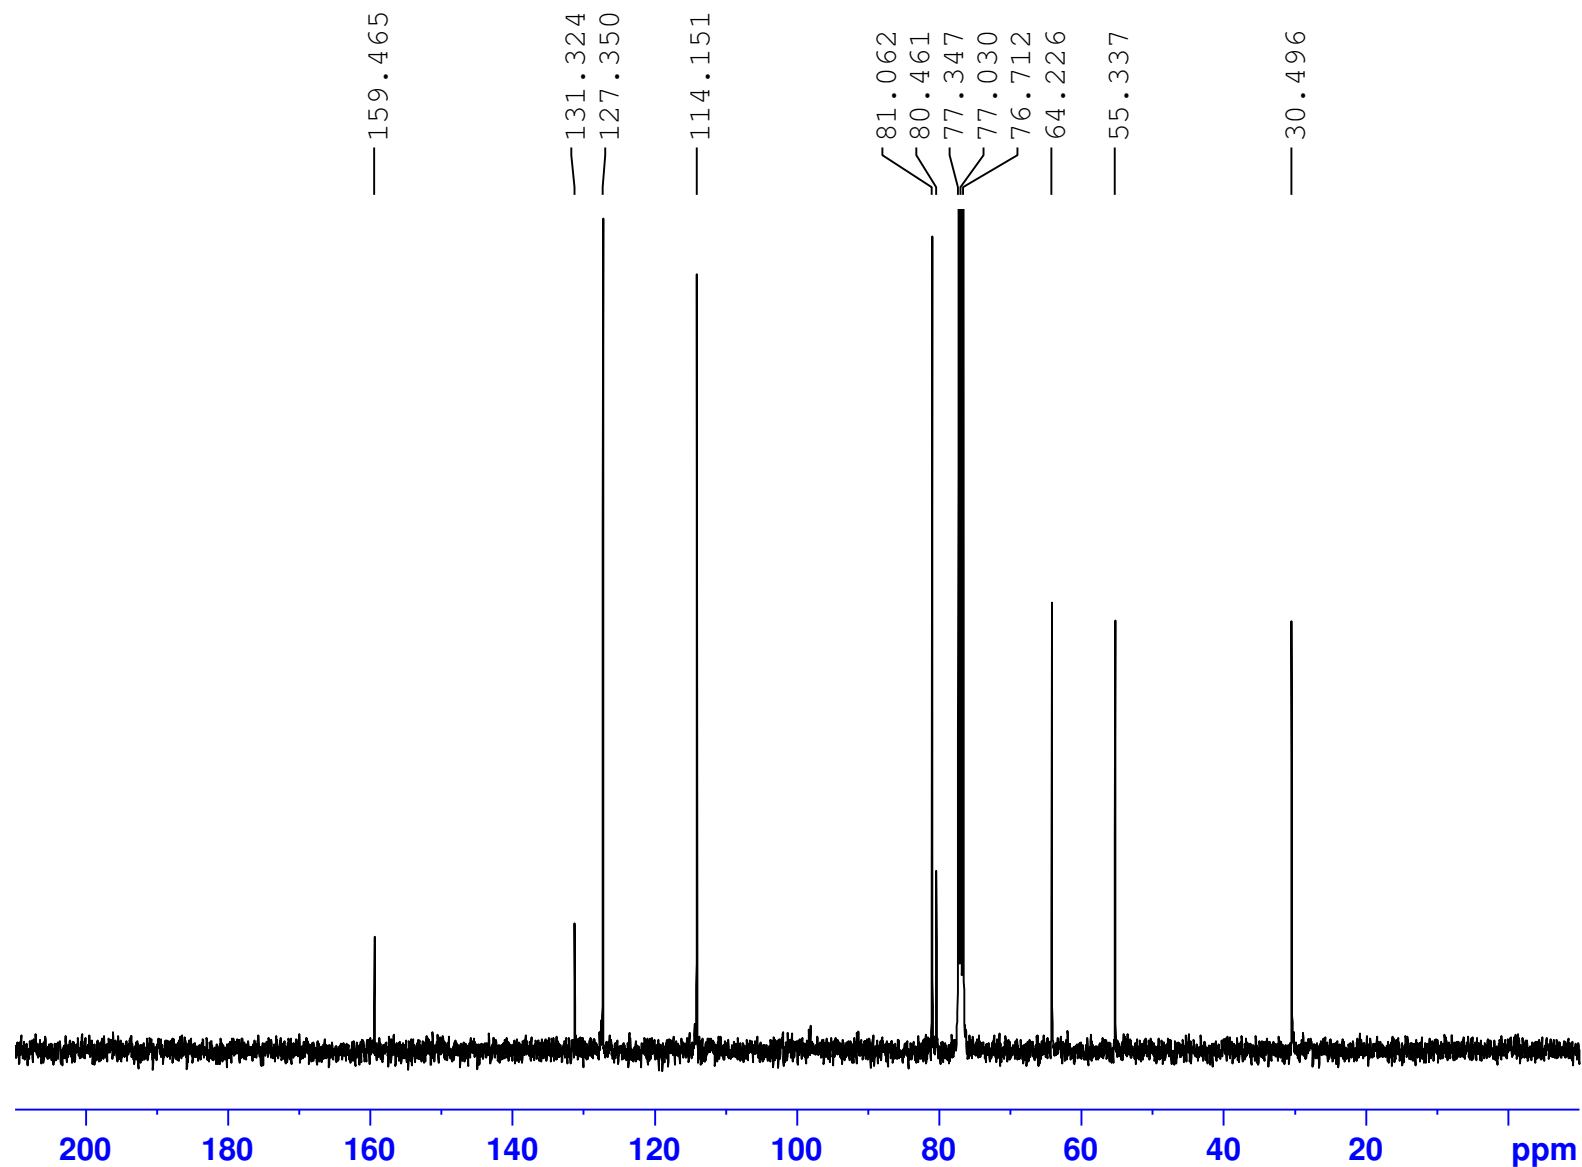


**Av-400A**

Current Data Parameters  
NAME Feb22-2022  
EXPNO 91  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20220223  
Time 3.04  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgpg30  
TD 32768  
SOLVENT CDCl<sub>3</sub>  
NS 1200  
DS 4  
SWH 26315.789 Hz  
FIDRES 0.803094 Hz  
AQ 0.6225920 sec  
RG 207.33  
DW 19.000 usec  
DE 6.50 usec  
TE 295.2 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 100.6942485 MHz  
NUC1 13C  
P1 9.60 usec  
PLW1 59.97900009 W

===== CHANNEL f2 =====  
SFO2 400.4119220 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 19.95299911 W  
PLW12 0.31176999 W  
PLW13 0.25253001 W

F2 - Processing parameters  
SI 16384  
SF 100.6831750 MHz  
WDW EM  
SSB 0  
LB 2.50 Hz  
GB 0  
PC 1.40