


060721_PPMS12179 #358 RT: 0.46 AV: 1 NL: 1.39E8
T: FTMS + p APCI corona Full ms [150.0000-900.0000]

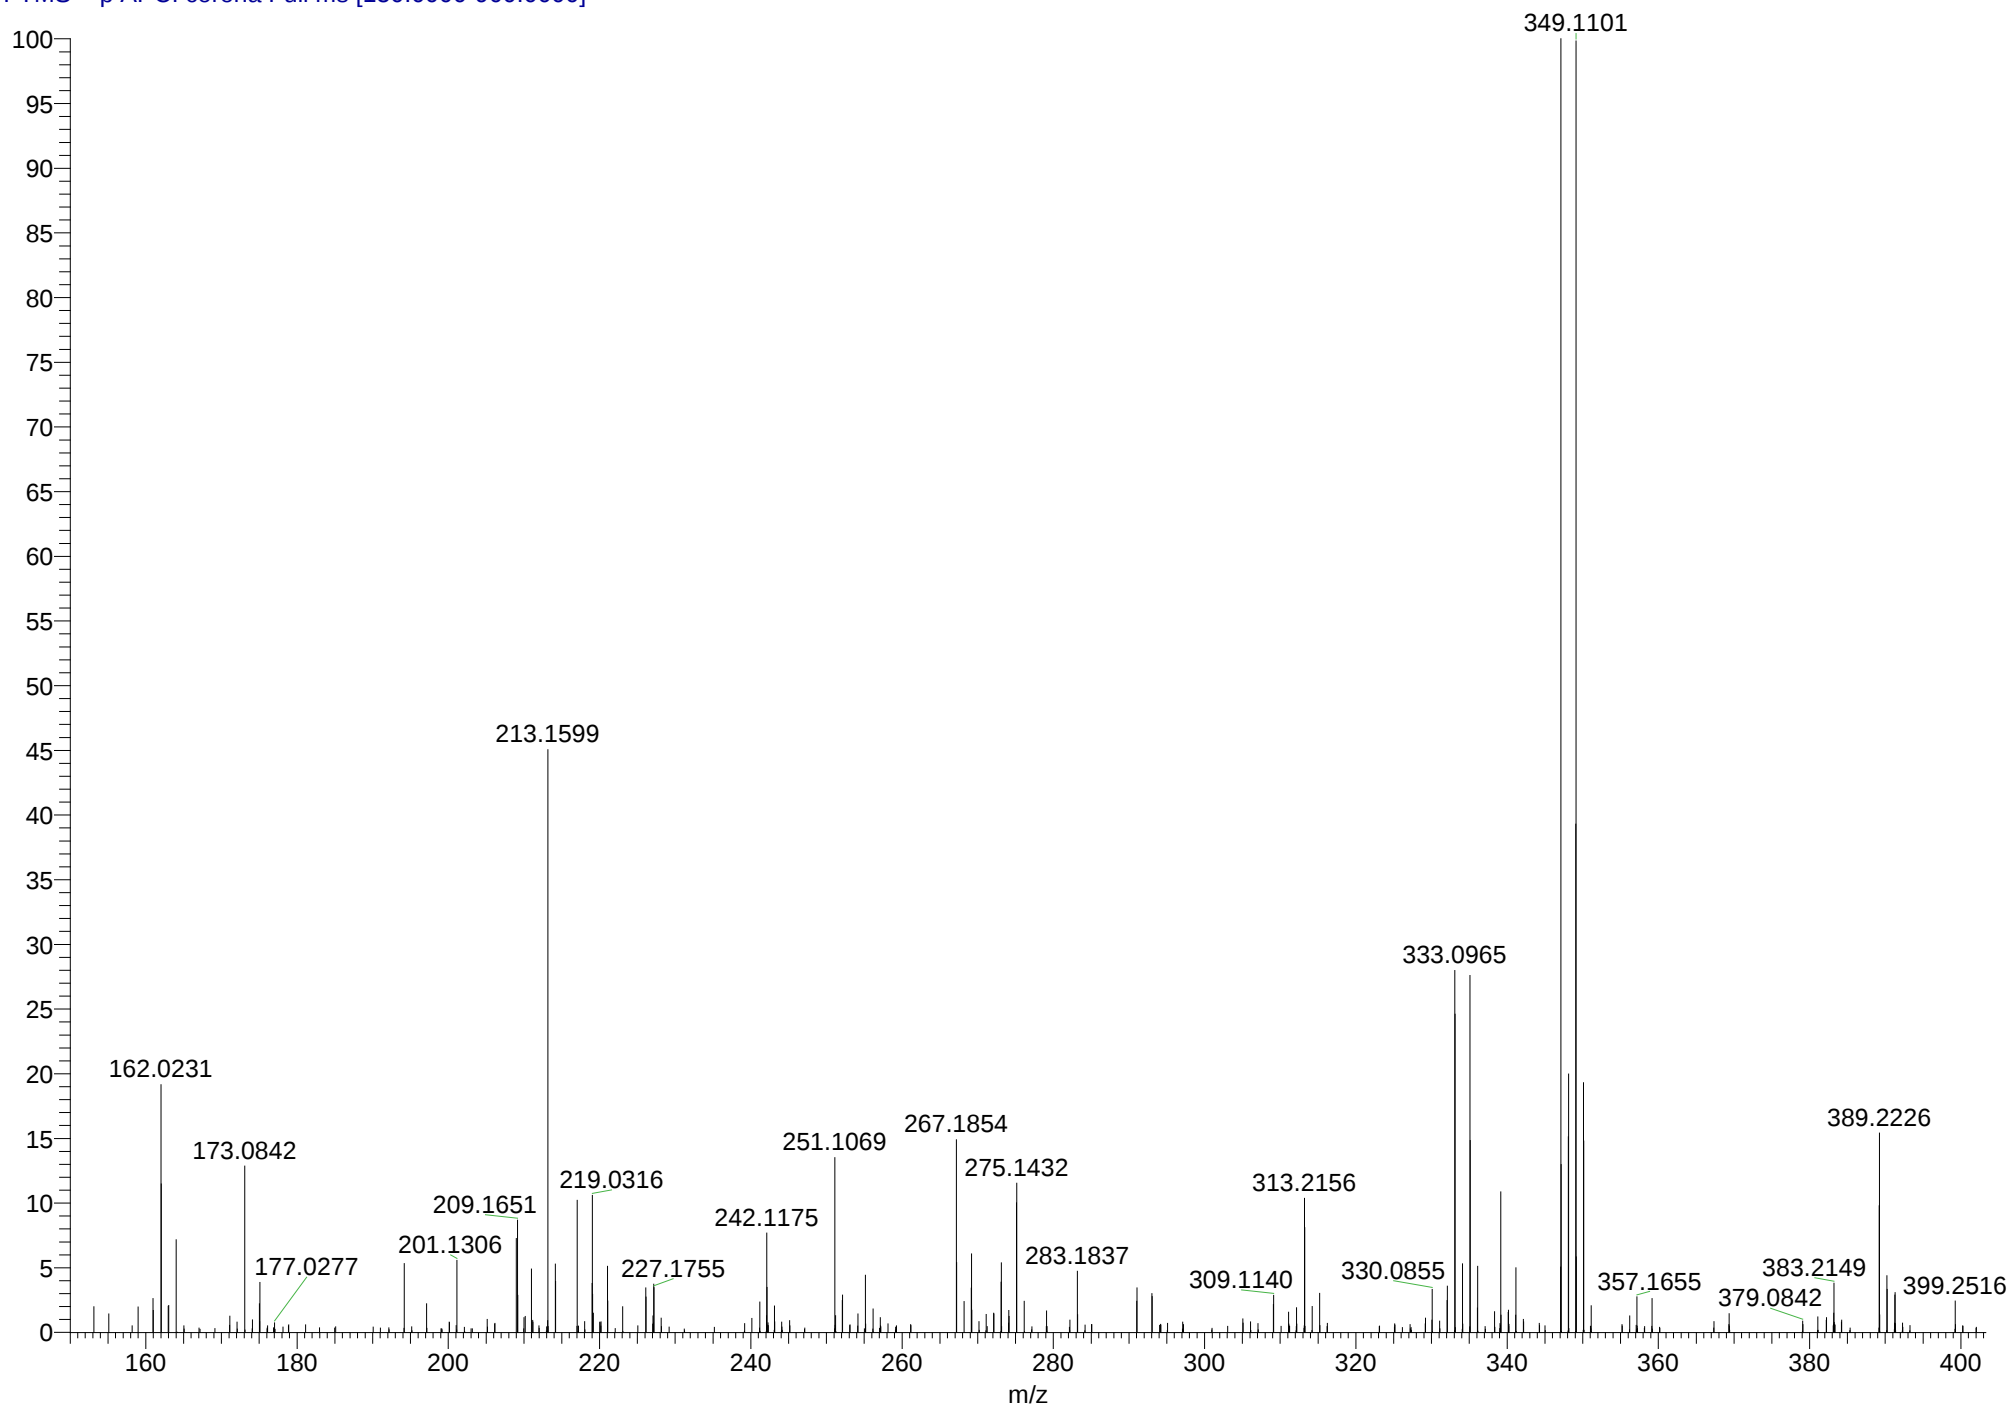

SAMPLE: PPMS12179 B.LANCASTER BL 042 02 PURE

EXPECTED ION NOT FOUND:

POSSIBLE FORMULA:

333.0965

	DBE	ERROR (PPM)	
1	C17 H22 N2 Br	7.5	0.412
2	C6 H22 O3 N8 Br	-0.5	-2.776
3	C14 H24 O3 N Br	3.0	3.092
4	C8 H24 O4 N5 Br	-1.0	-4.118
5	C12 H22 O2 N4 Br	3.5	4.435

347.1120

1	C18 H24 N2 Br	7.5	0.262
2	C7 H24 O3 N8 Br	-0.5	-2.926
3	C15 H26 O3 N Br	3.0	2.942
4	C9 H26 O4 N5 Br	-1.0	-4.268
5	C13 H24 O2 N4 Br	3.5	4.285

ANALYSIS RUN USING: THERMO FISHER Q-EXACTIVE PLUS (APCI POSITIVE/APCI NEGATIVE) XCALIBUR