



BL-491
BL-491 7 (0.171)

16-May-2024
1: TOF MS ES+
928.6699 399

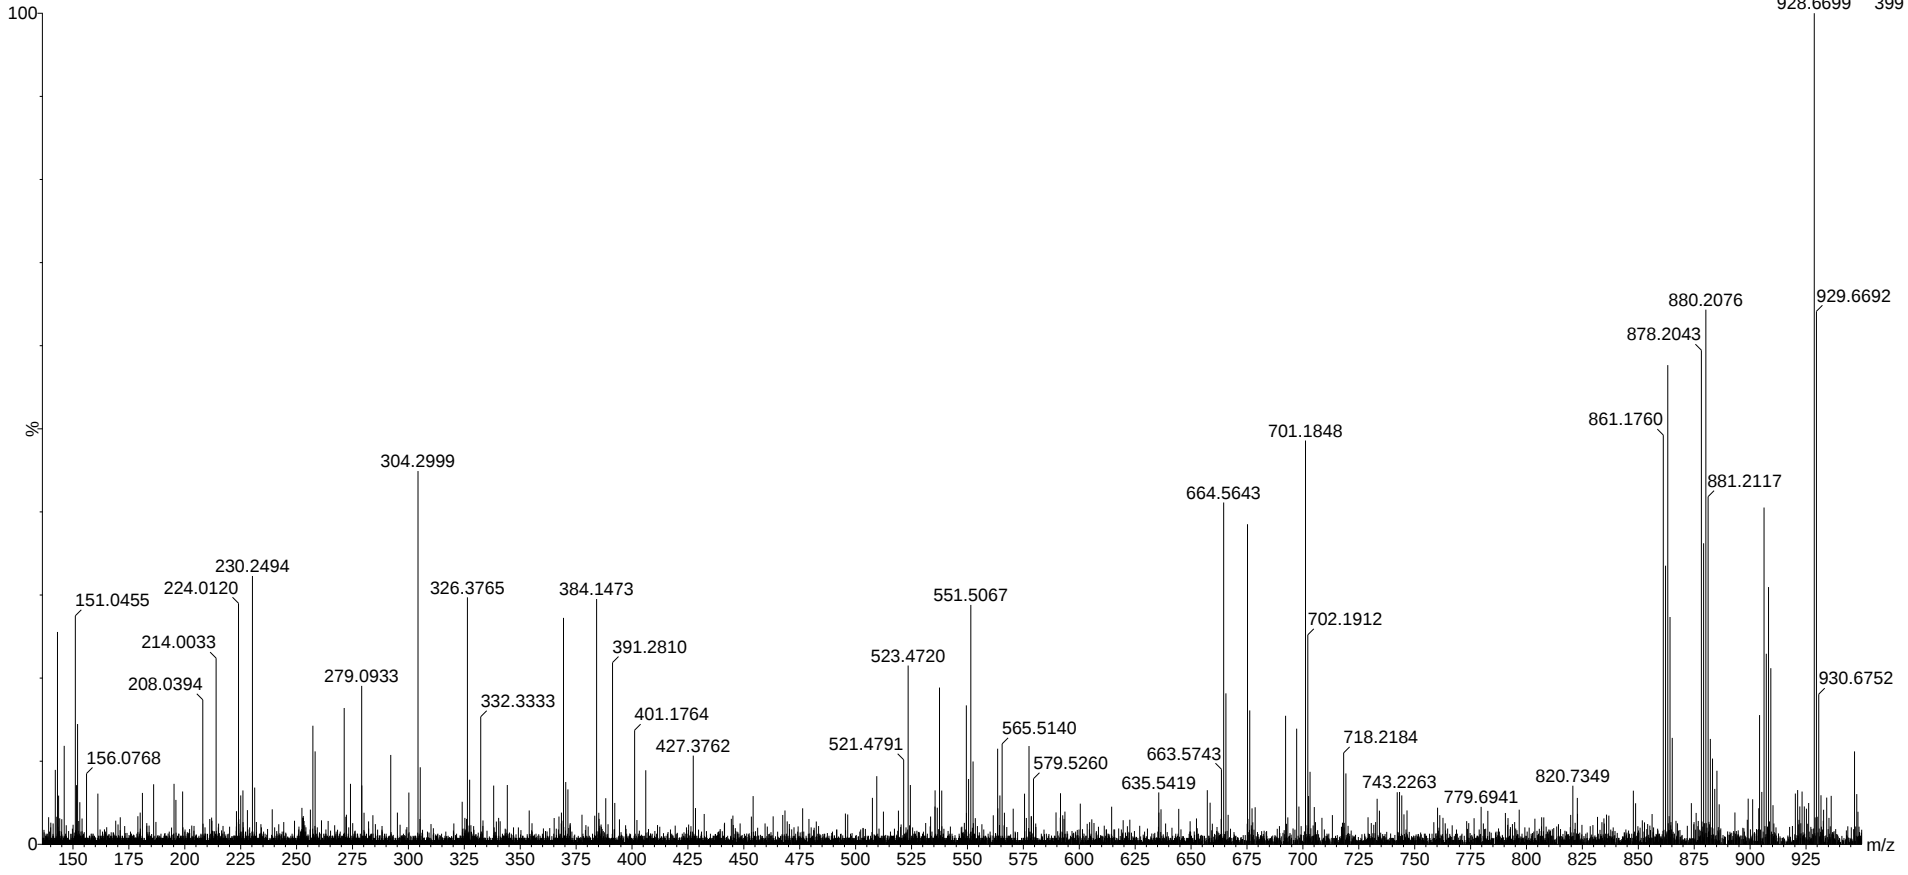

BL-491
BL-491 7 (0.171)

16-May-2024
1: TOF MS ES+
399

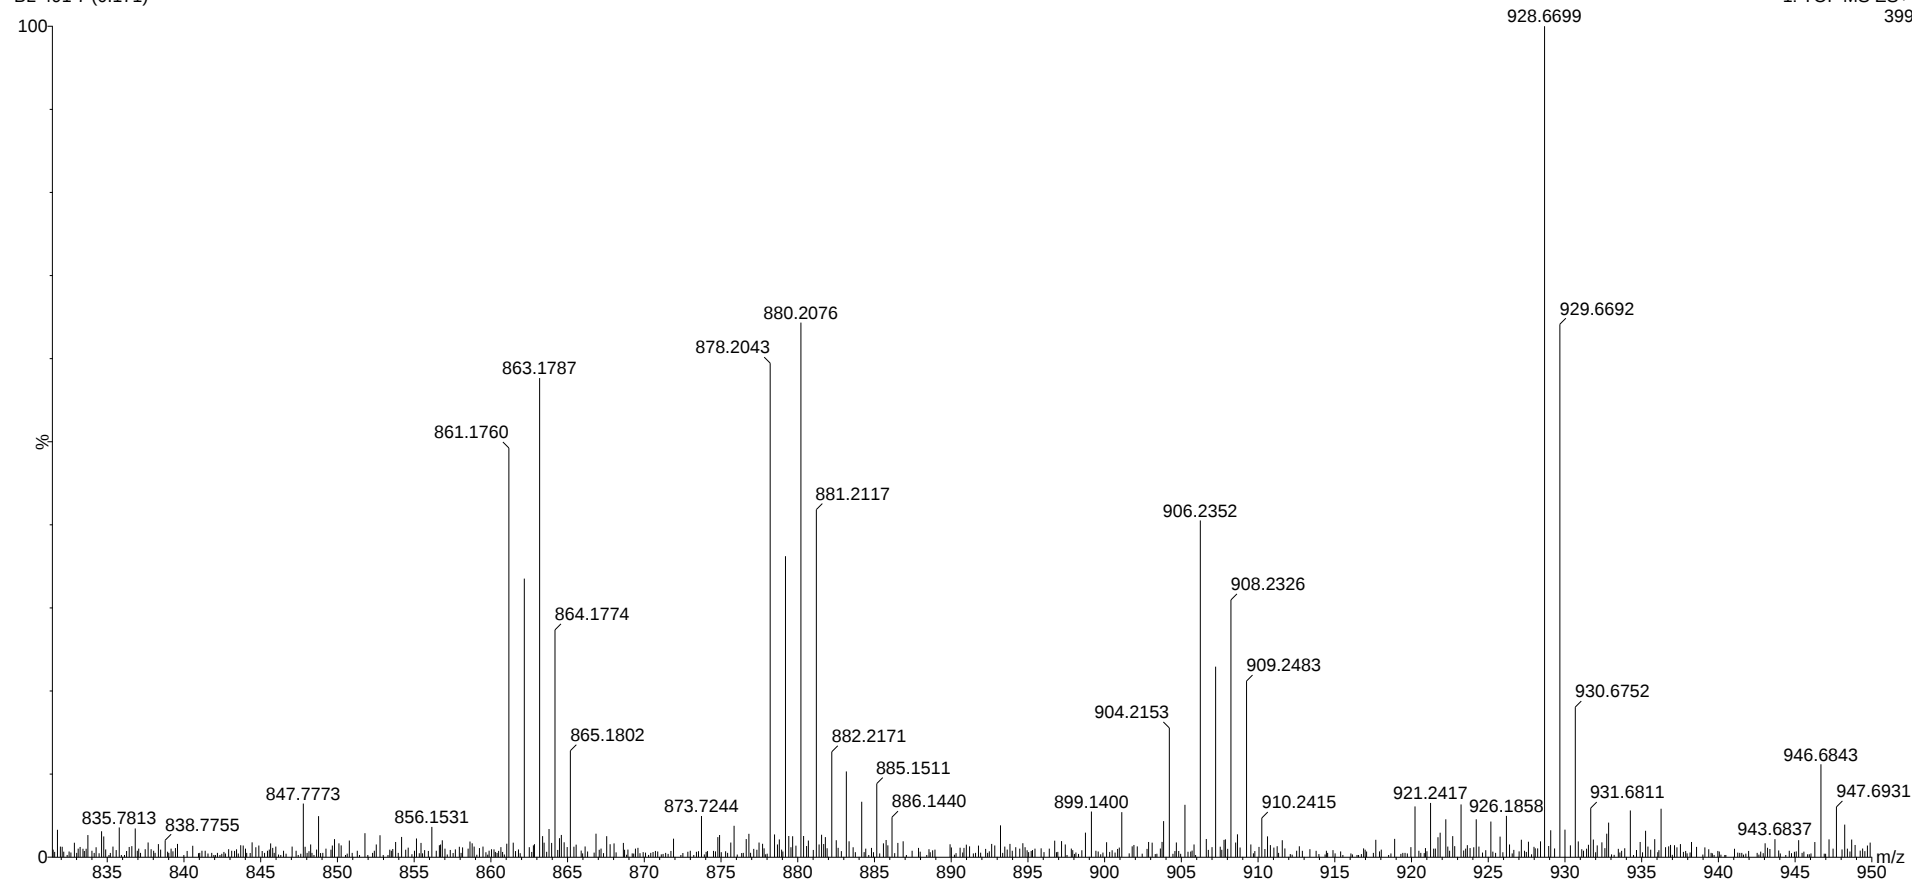

Elemental Composition Report for [M+H]⁺

Single Mass Analysis

Tolerance = 5.0 PPM / DBE: min = -1.5, max = 100.0

Element prediction: Off

Number of isotope peaks used for i-FIT = 3

Monoisotopic Mass, Even Electron Ions

187 formula(e) evaluated with 1 results within limits (all results (up to 1000) for each mass)

Elements Used:

C: 10-80 H: 0-160 O: 1-10 P: 1-1 Br: 0-1

Minimum: -1.5

Maximum: 5.0 5.0 100.0

Mass	Calc. Mass	mDa	PPM	DBE	i-FIT	i-FIT (Norm)	Formula
861.1760	861.1769	-0.9	-1.0	35.5	45.4	0.0	C54 H39 O4 P Br