



BL394
BL394 24 (0.619)

21-Apr-2023
1: TOF MS ES+
1.23e3

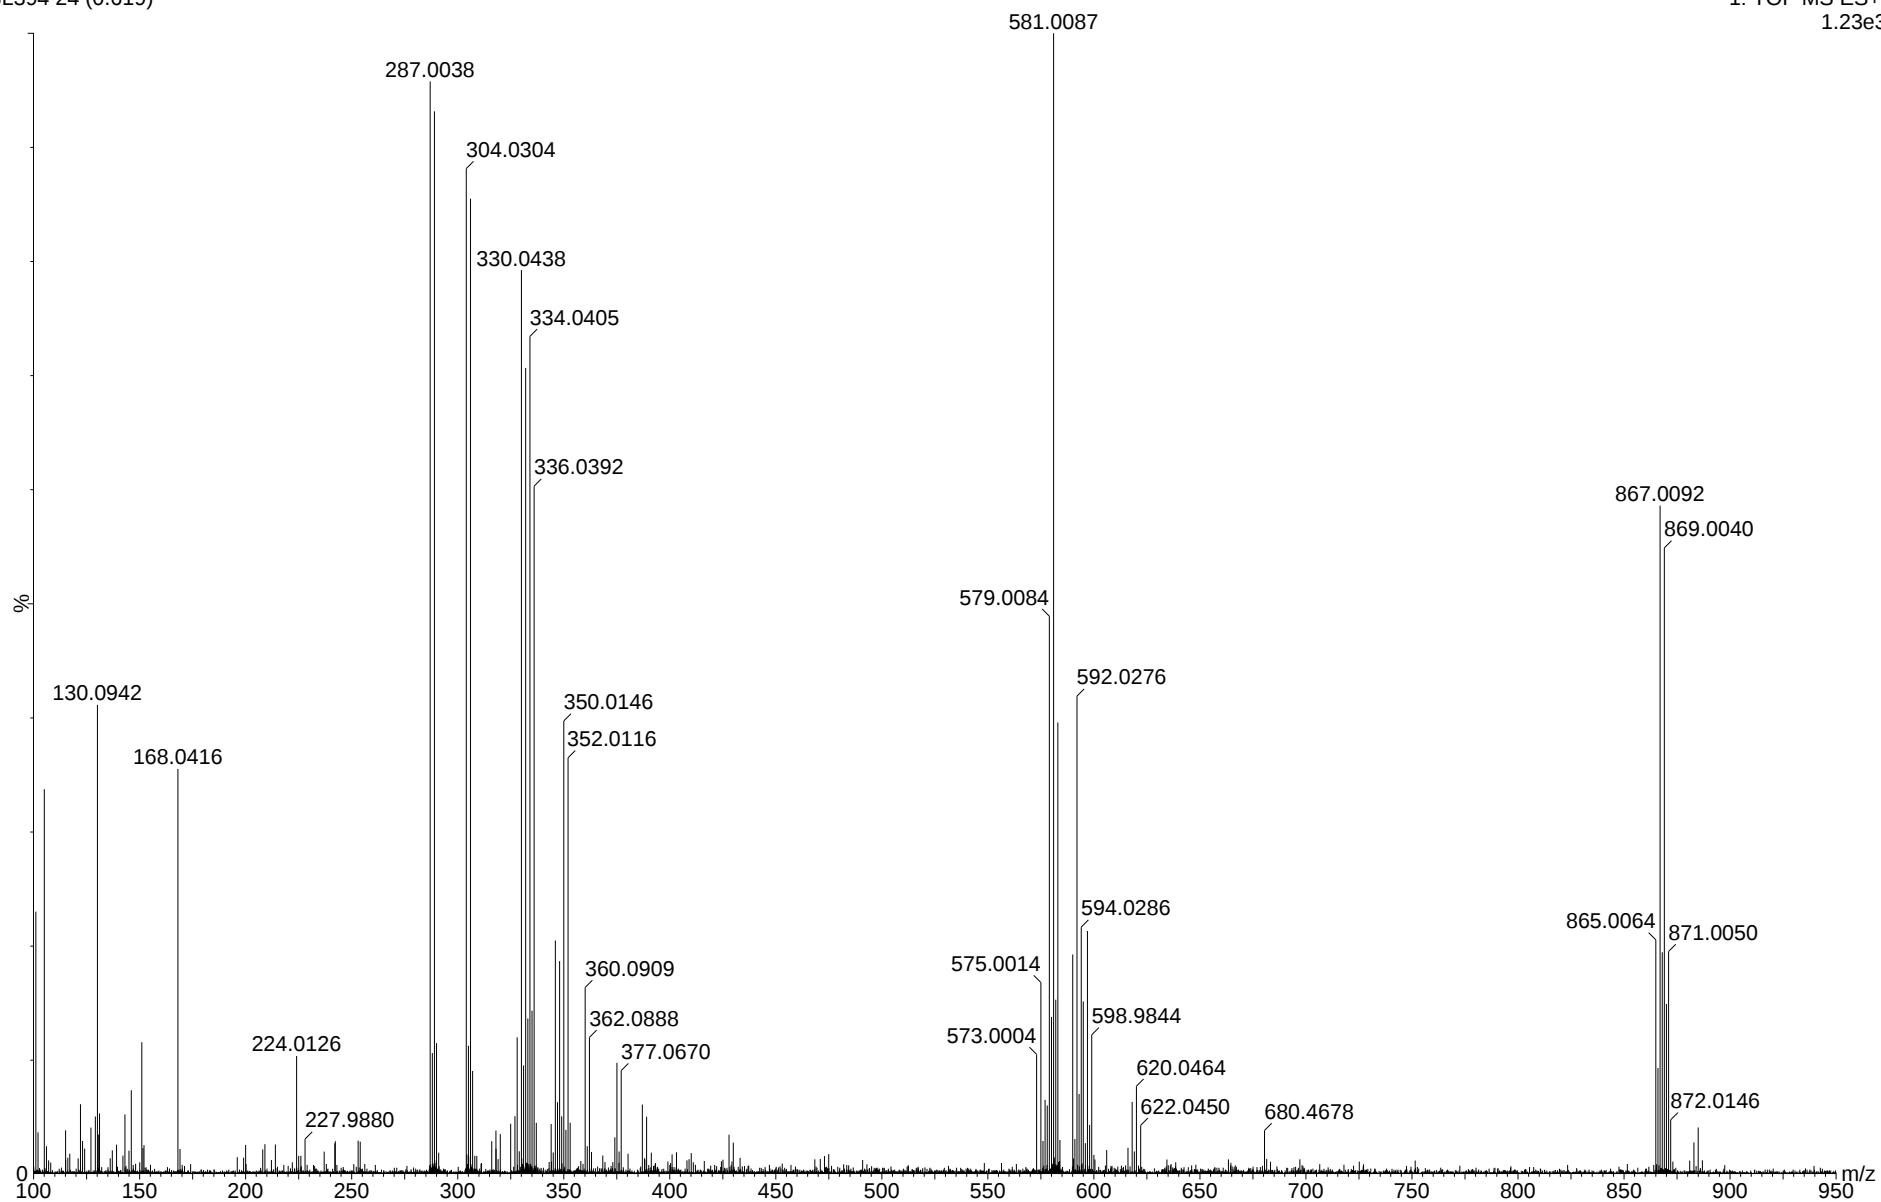

BL394
BL394 24 (0.619)

21-Apr-2023
1: TOF MS ES+
1.18e3

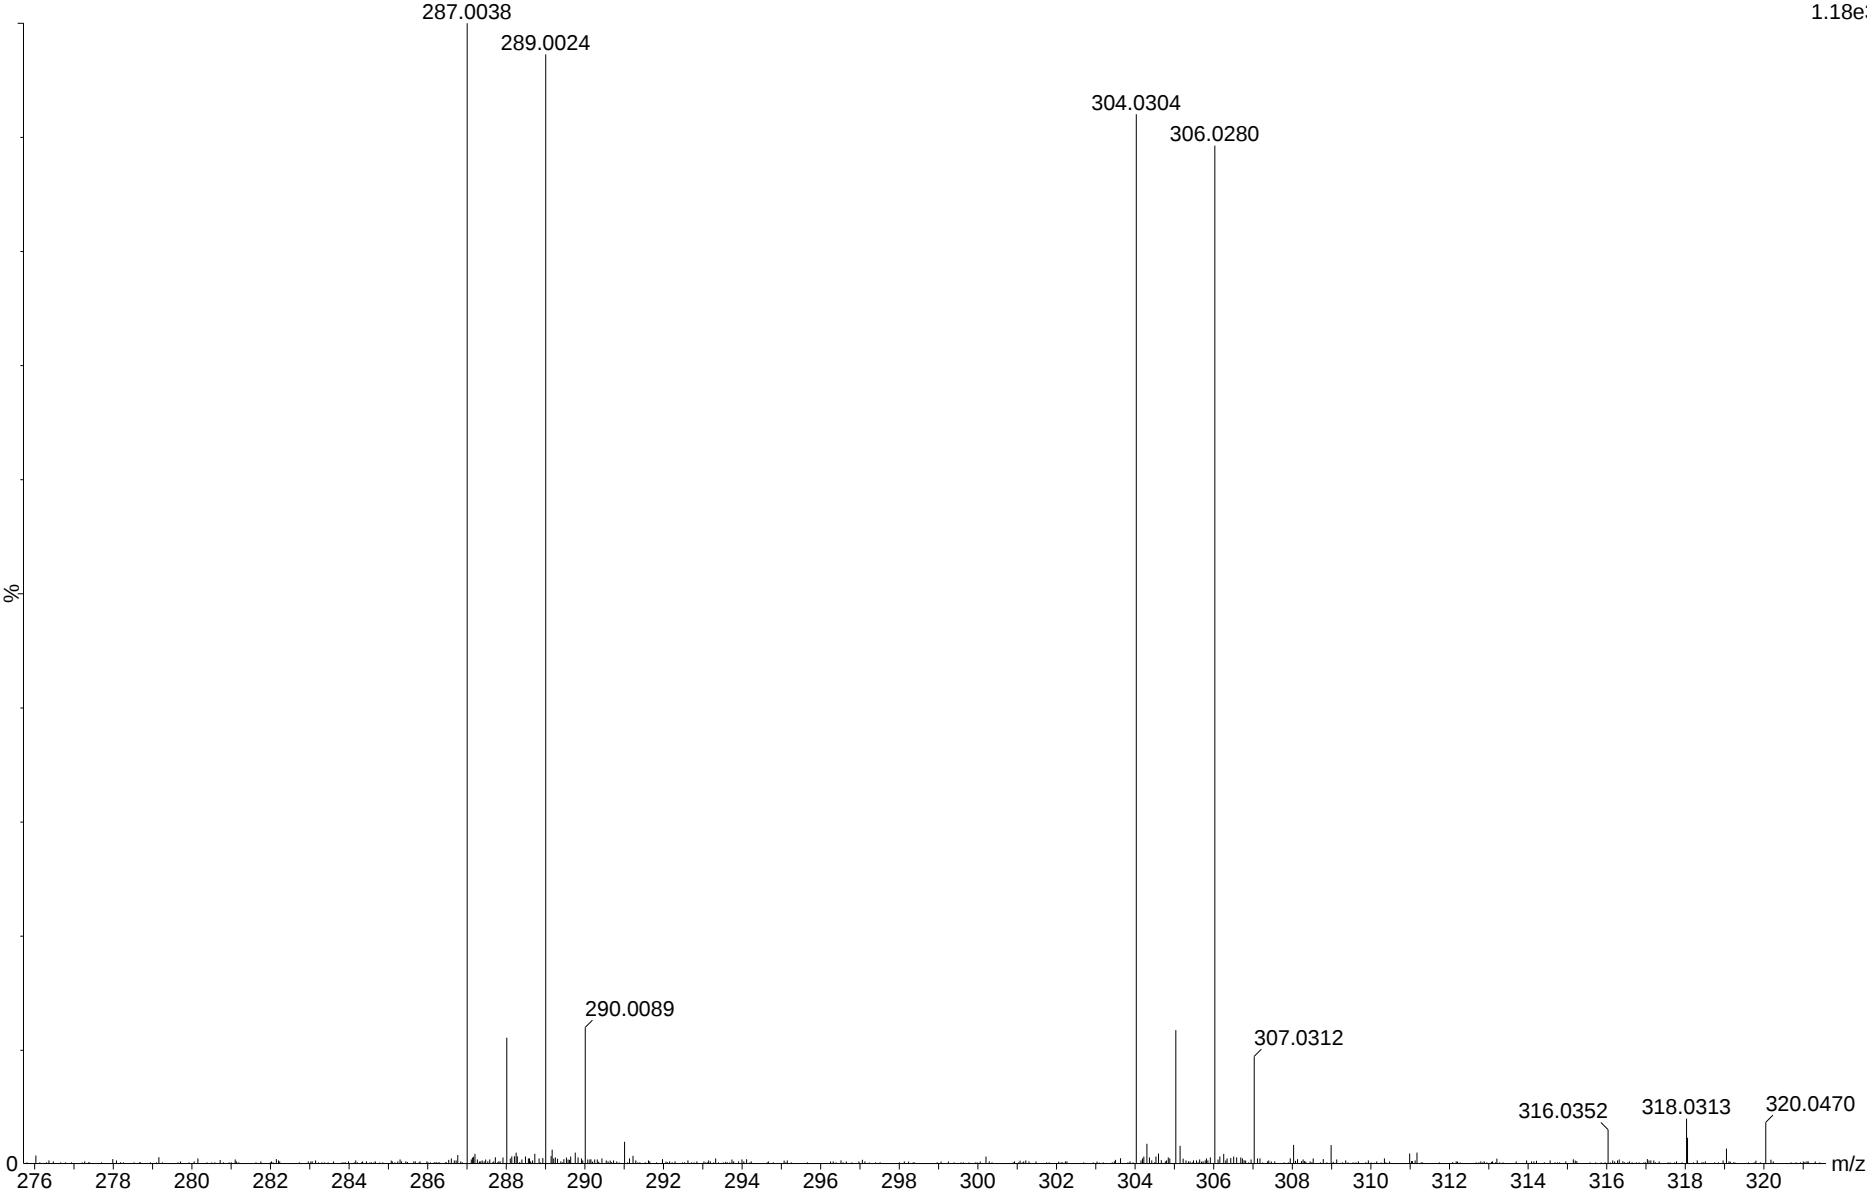

Elemental Composition Report for [M+H]⁺

Single Mass Analysis

Tolerance = 5.0 PPM / DBE: min = -1.5, max = 100.0

Element prediction: Off

Number of isotope peaks used for i-FIT = 3

Monoisotopic Mass, Even Electron Ions

31 formula(e) evaluated with 1 results within limits (all results (up to 1000) for each mass)

Elements Used:

C: 8-12 H: 0-100 O: 0-15 Br: 1-1 P: 1-2

		Minimum:					-1.5
		Maximum:		5.0	5.0	100.0	
Mass	Calc. Mass	mDa	PPM	DBE	i-FIT	i-FIT (Norm)	Formula
287.0038	287.0048	-1.0	-3.5	0.5	165.5	0.0	C8 H17 O4 Br P