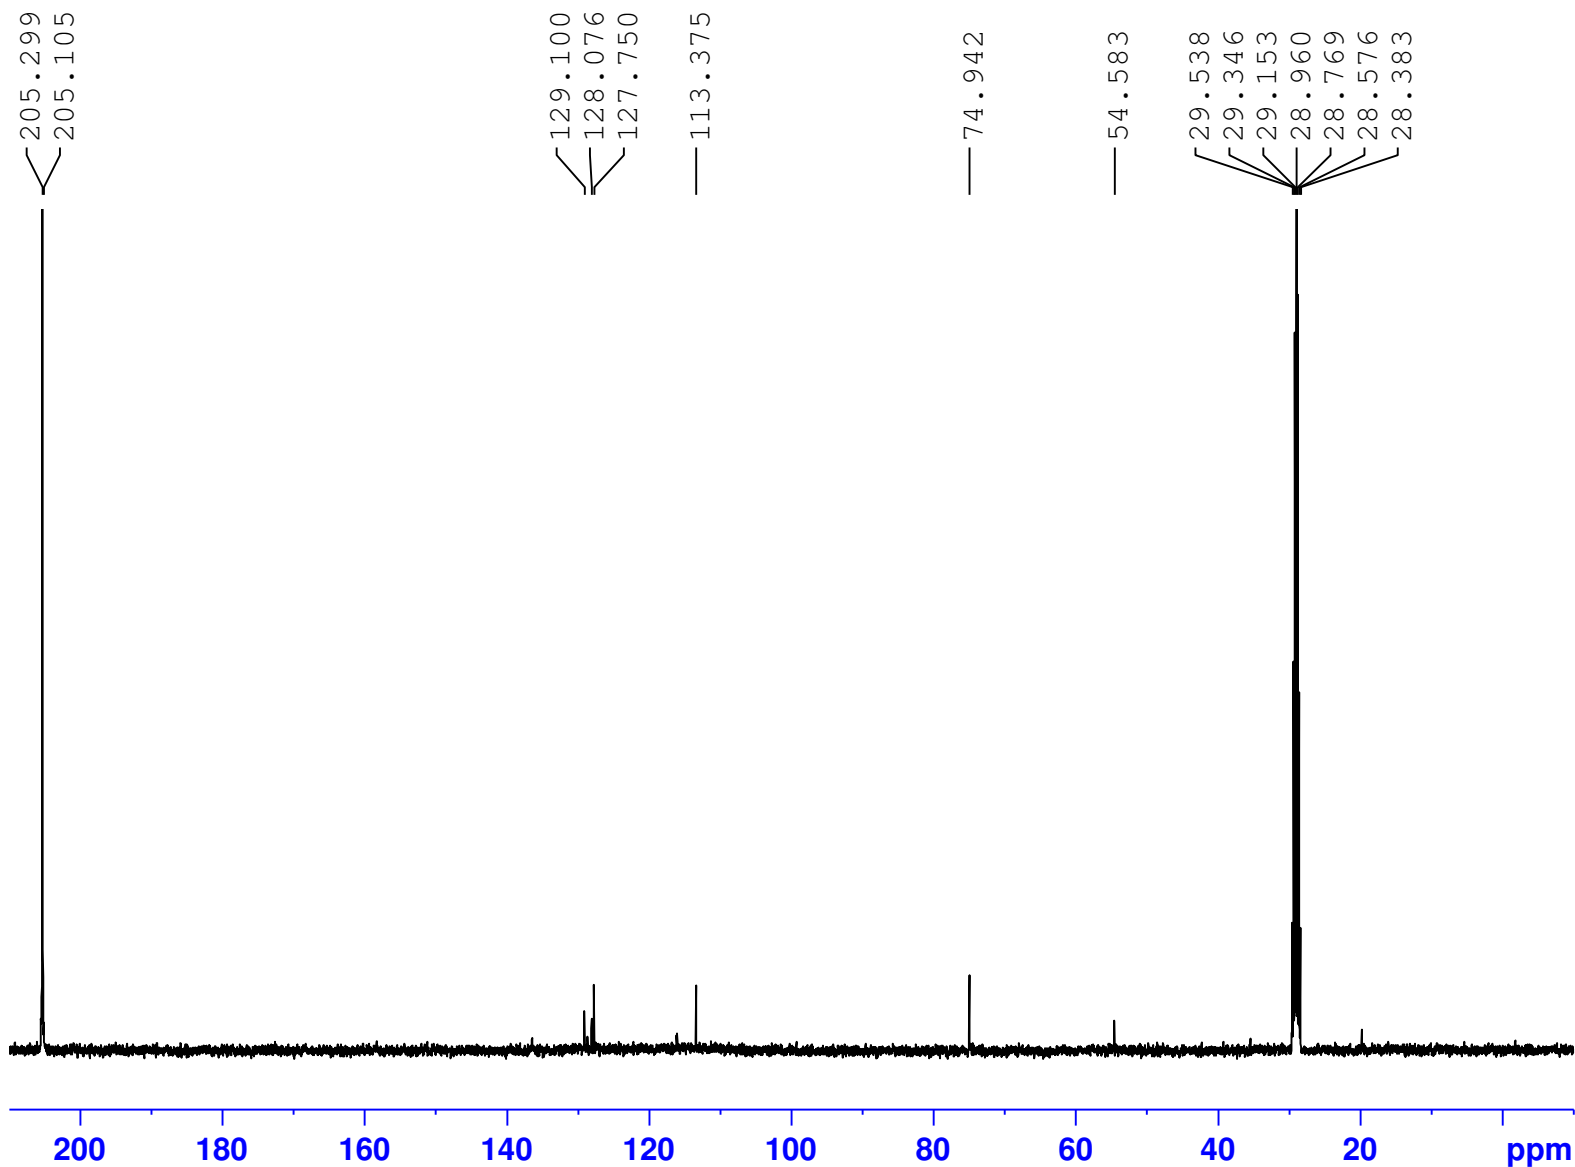


Av400B

Current Data Parameters
NAME Sep14-2022
EXPNO 331
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220914
Time 19.14
INSTRUM spect
PROBHD 5 mm PABBI 1H/
PULPROG zgpg30
TD 32768
SOLVENT Acetone
NS 352
DS 4
SWH 28409.092 Hz
FIDRES 0.866977 Hz
AQ 0.5767168 sec
RG 51.12
DW 17.600 usec
DE 6.50 usec
TE 295.2 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 100.6716168 MHz
NUC1 13C
P1 13.00 usec
PLW1 109.90000153 W

===== CHANNEL f2 =====
SFO2 400.3220016 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 7.24440002 W
PLW12 0.08502100 W
PLW13 0.06886700 W

F2 - Processing parameters
SI 32768
SF 100.6605440 MHz
WDW EM
SSB 0
LB 2.00 Hz
GB 0
PC 1.20