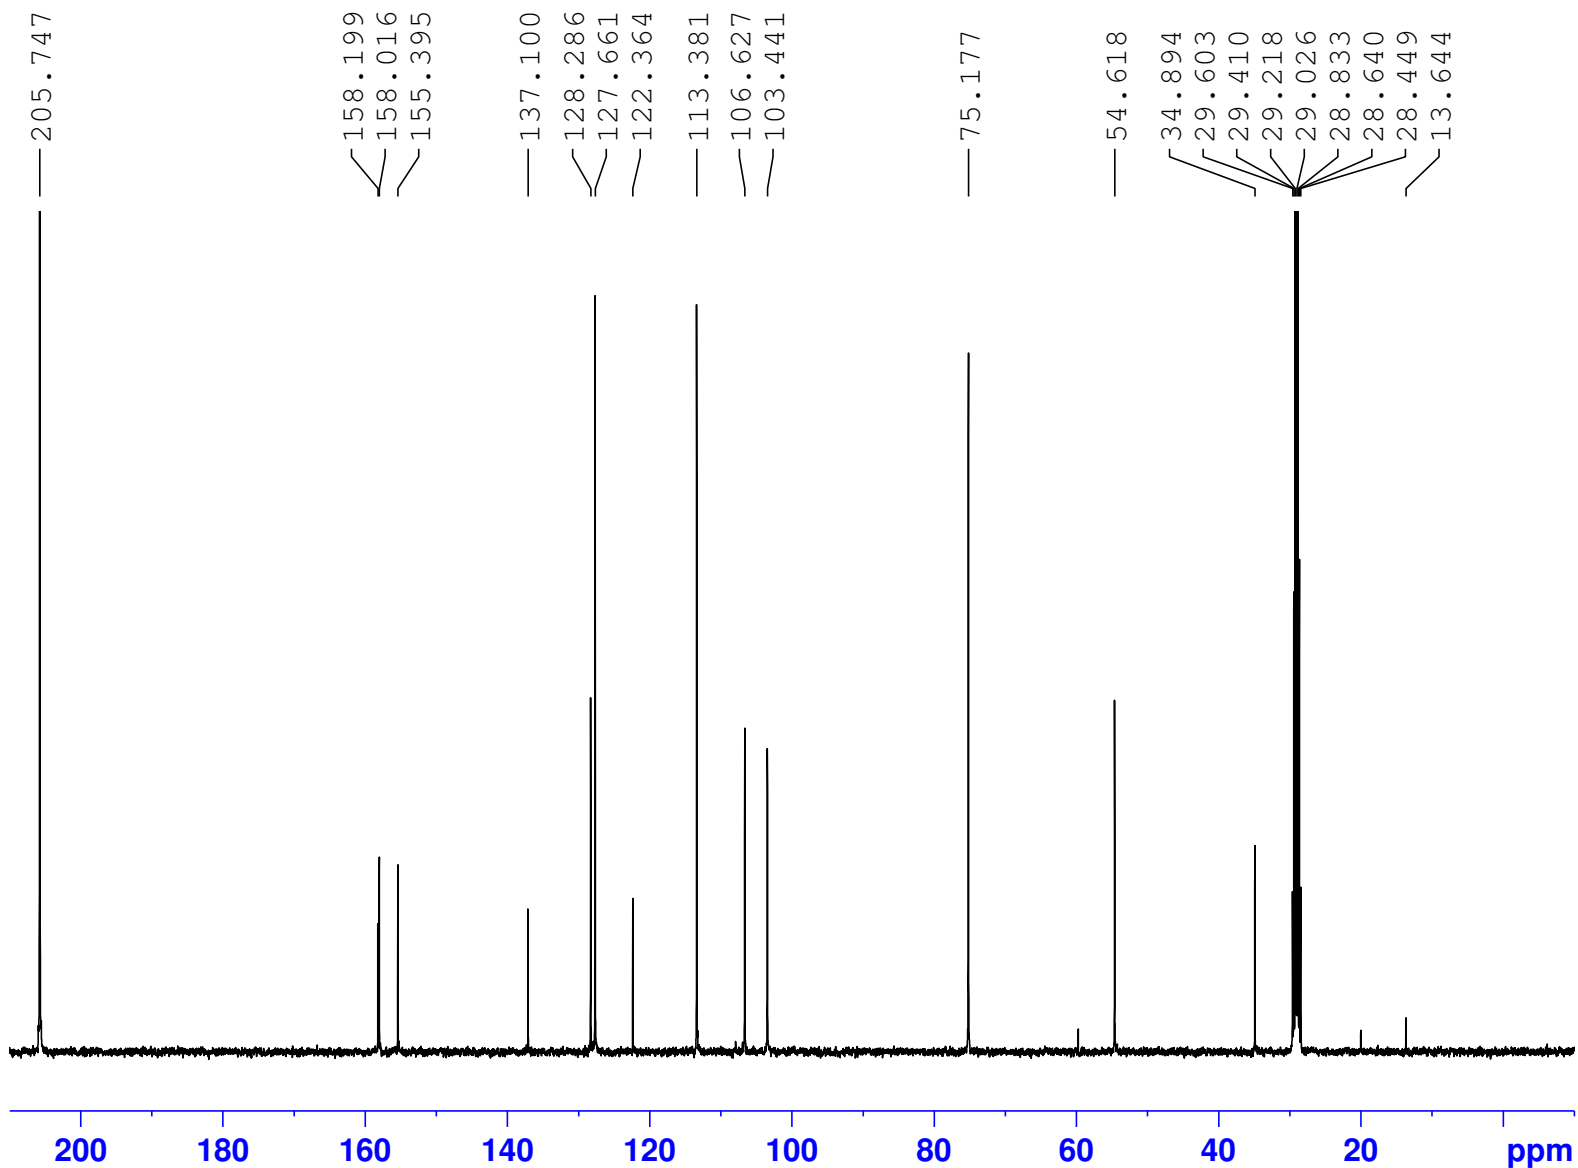


Av400B

Current Data Parameters
NAME Oct09-2023
EXPNO 71
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231009
Time 17.03 h
INSTRUM spect
PROBHD Z108618_0625 (
PULPROG zgpg30
TD 32768
SOLVENT Acetone
NS 352
DS 4
SWH 28409.092 Hz
FIDRES 1.733953 Hz
AQ 0.5767168 sec
RG 199.76
DW 17.600 usec
DE 6.50 usec
TE 295.9 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1
SFO1 100.6716168 MHz
NUC1 13C
P0 3.27 usec
P1 9.80 usec
PLW1 50.11899948 W
SFO2 400.3220016 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 20.00000000 W
PLW12 0.29877001 W
PLW13 0.24200000 W

F2 - Processing parameters
SI 32768
SF 100.6605440 MHz
WDW EM
SSB 0
LB 2.00 Hz
GB 0
PC 1.20