


RP184 -2 B(OArF3)3
B11.ucl CDCl3 {U:\400} tds 16

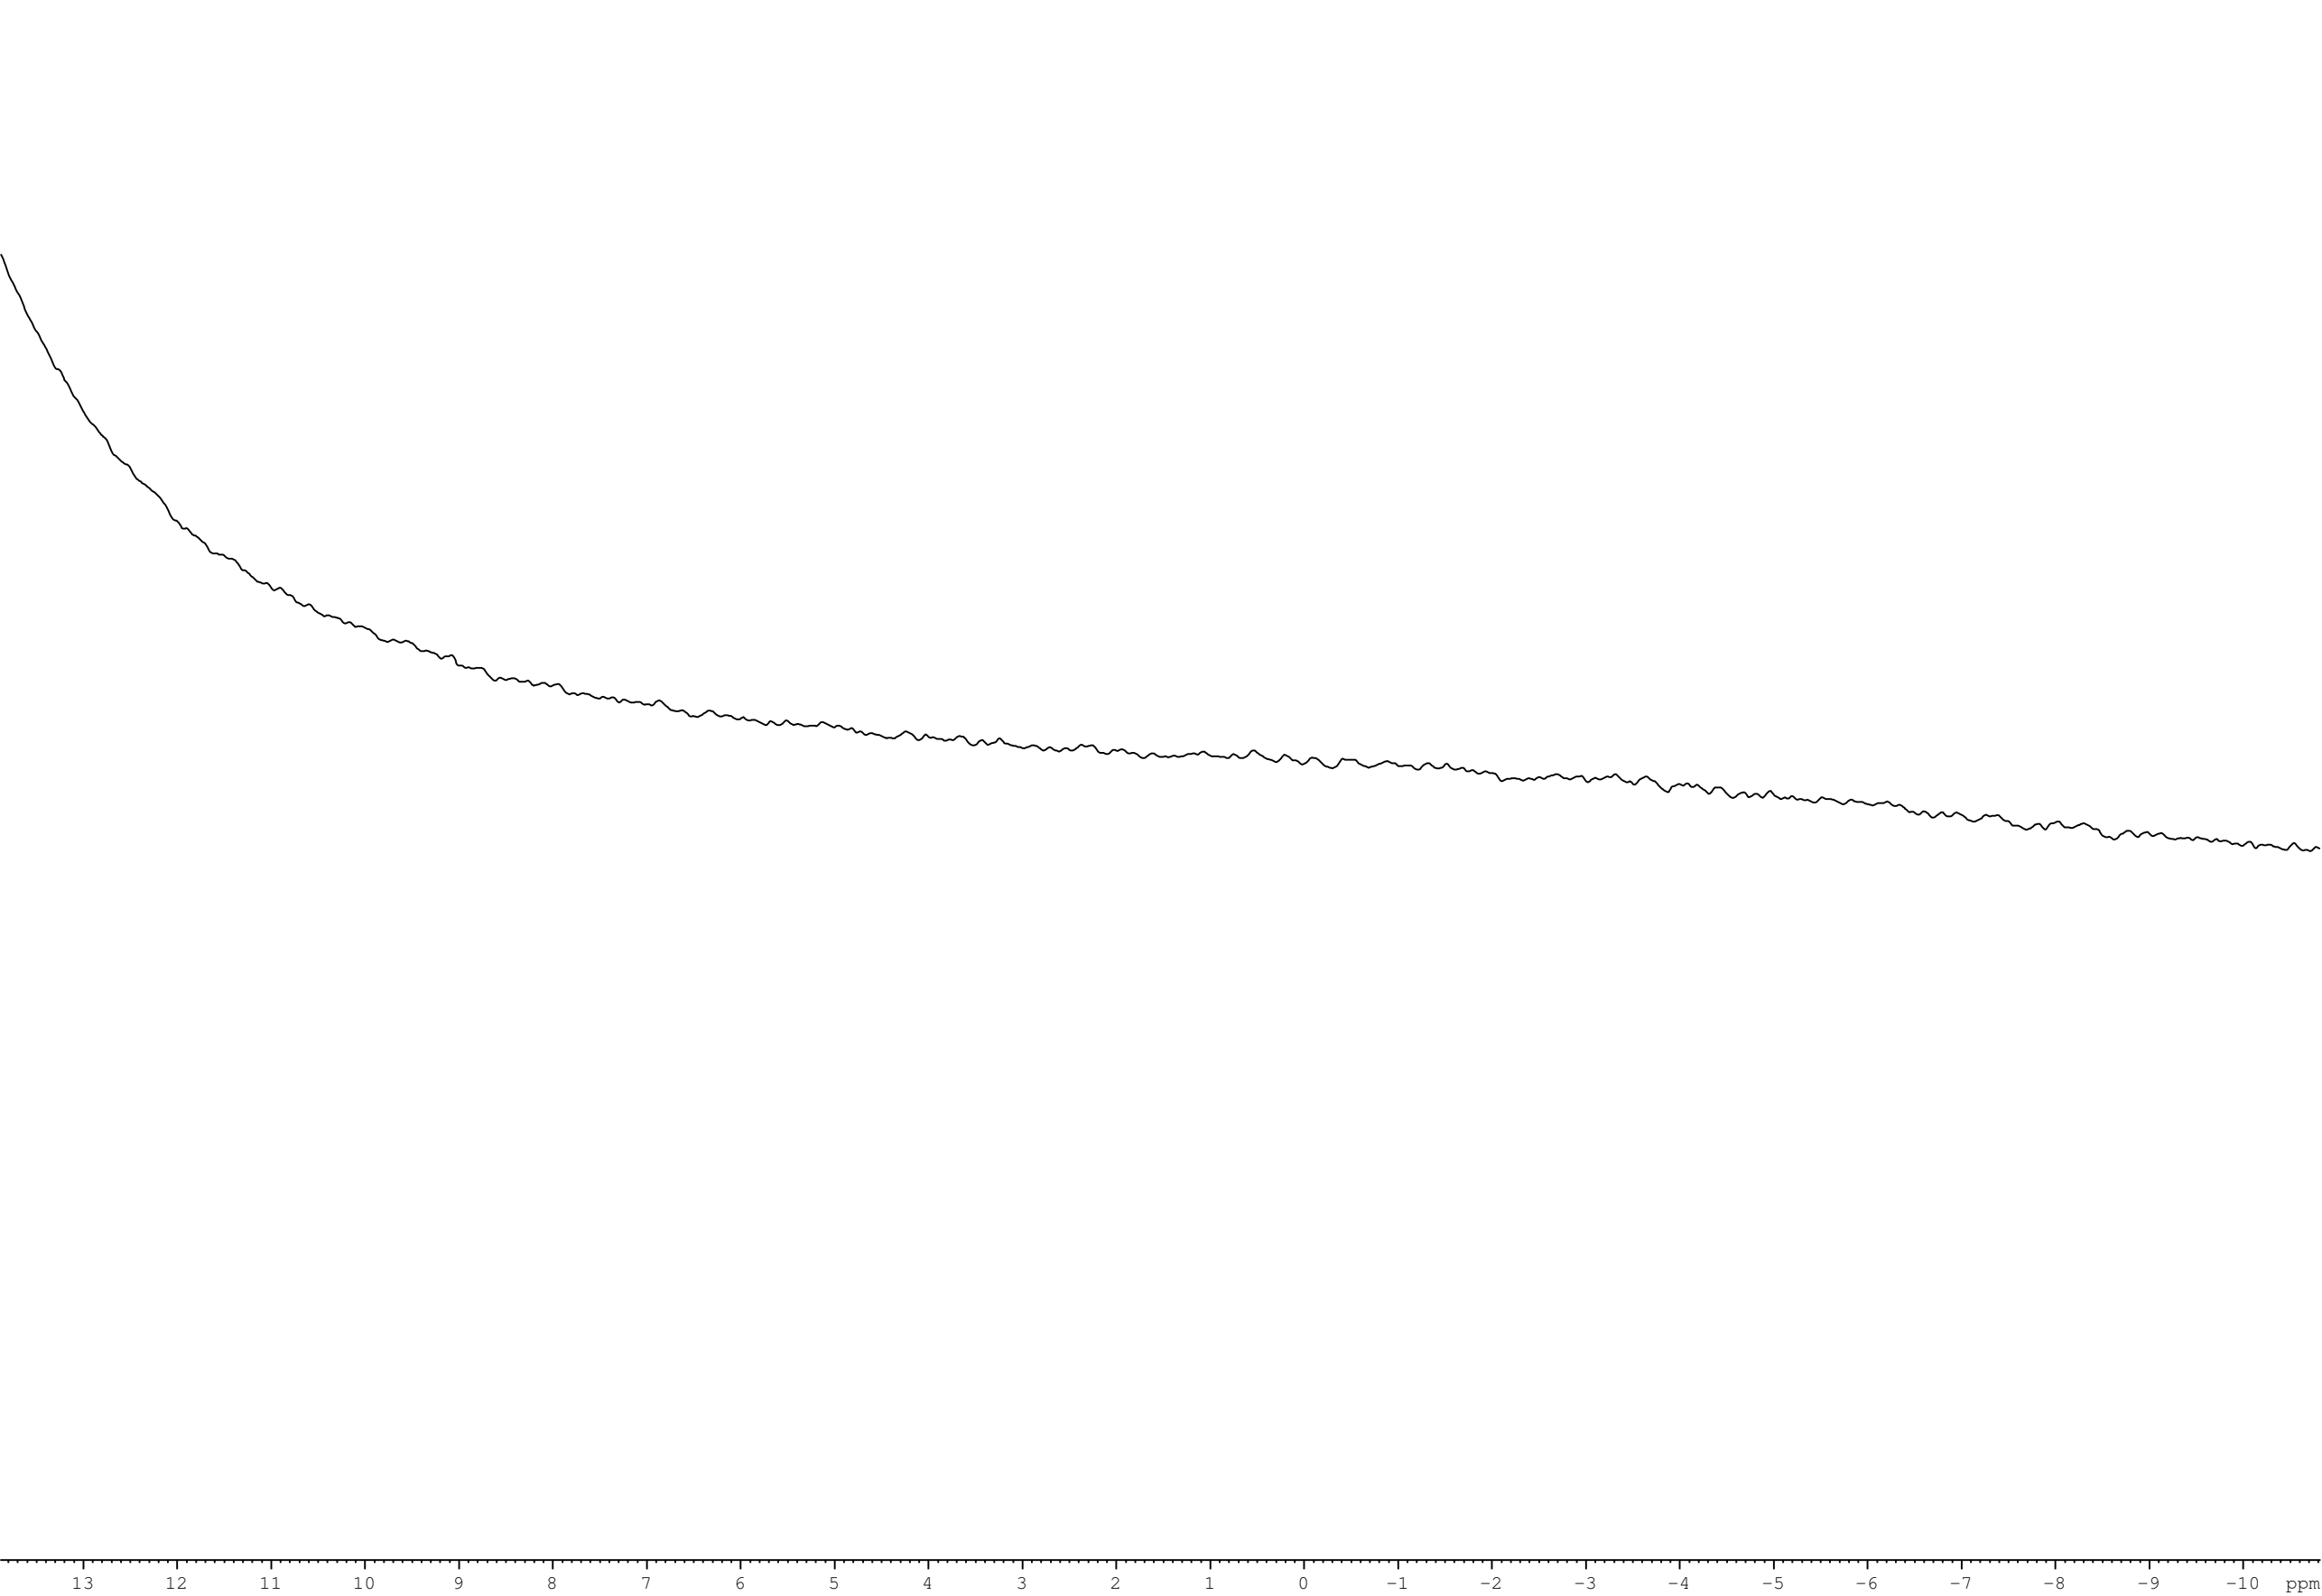

Current Data Parameters
NAME RP184 - 2
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20220322
Time 1.02
INSTRUM av400
PROBHD 5 mm PABBO BB/
PULPROG zg
TD 102034
SOLVENT CDCl3
NS 64
DS 0
SWH 51020.406 Hz
FIDRES 0.500033 Hz
AQ 0.9999332 s
RG 1620
DW 9.800 us
DE 6.50 us
TE 294.5 K
D1 1.00000000 s
TD0 1

===== CHANNEL f1 =====
SFO1 128.3673381 MHz
NUC1 11B
P1 82.50 us
PLW1 22.00000000 W

F2 - Processing parameters
SI 32768
SF 128.3679800 MHz
WDW EM
SSB 0
LB 10.00 Hz
GB 0
PC 1.00