


RP107 distilled CDCl3  
B11zgbs.ucl CDCl3 {U:\400} tds 5

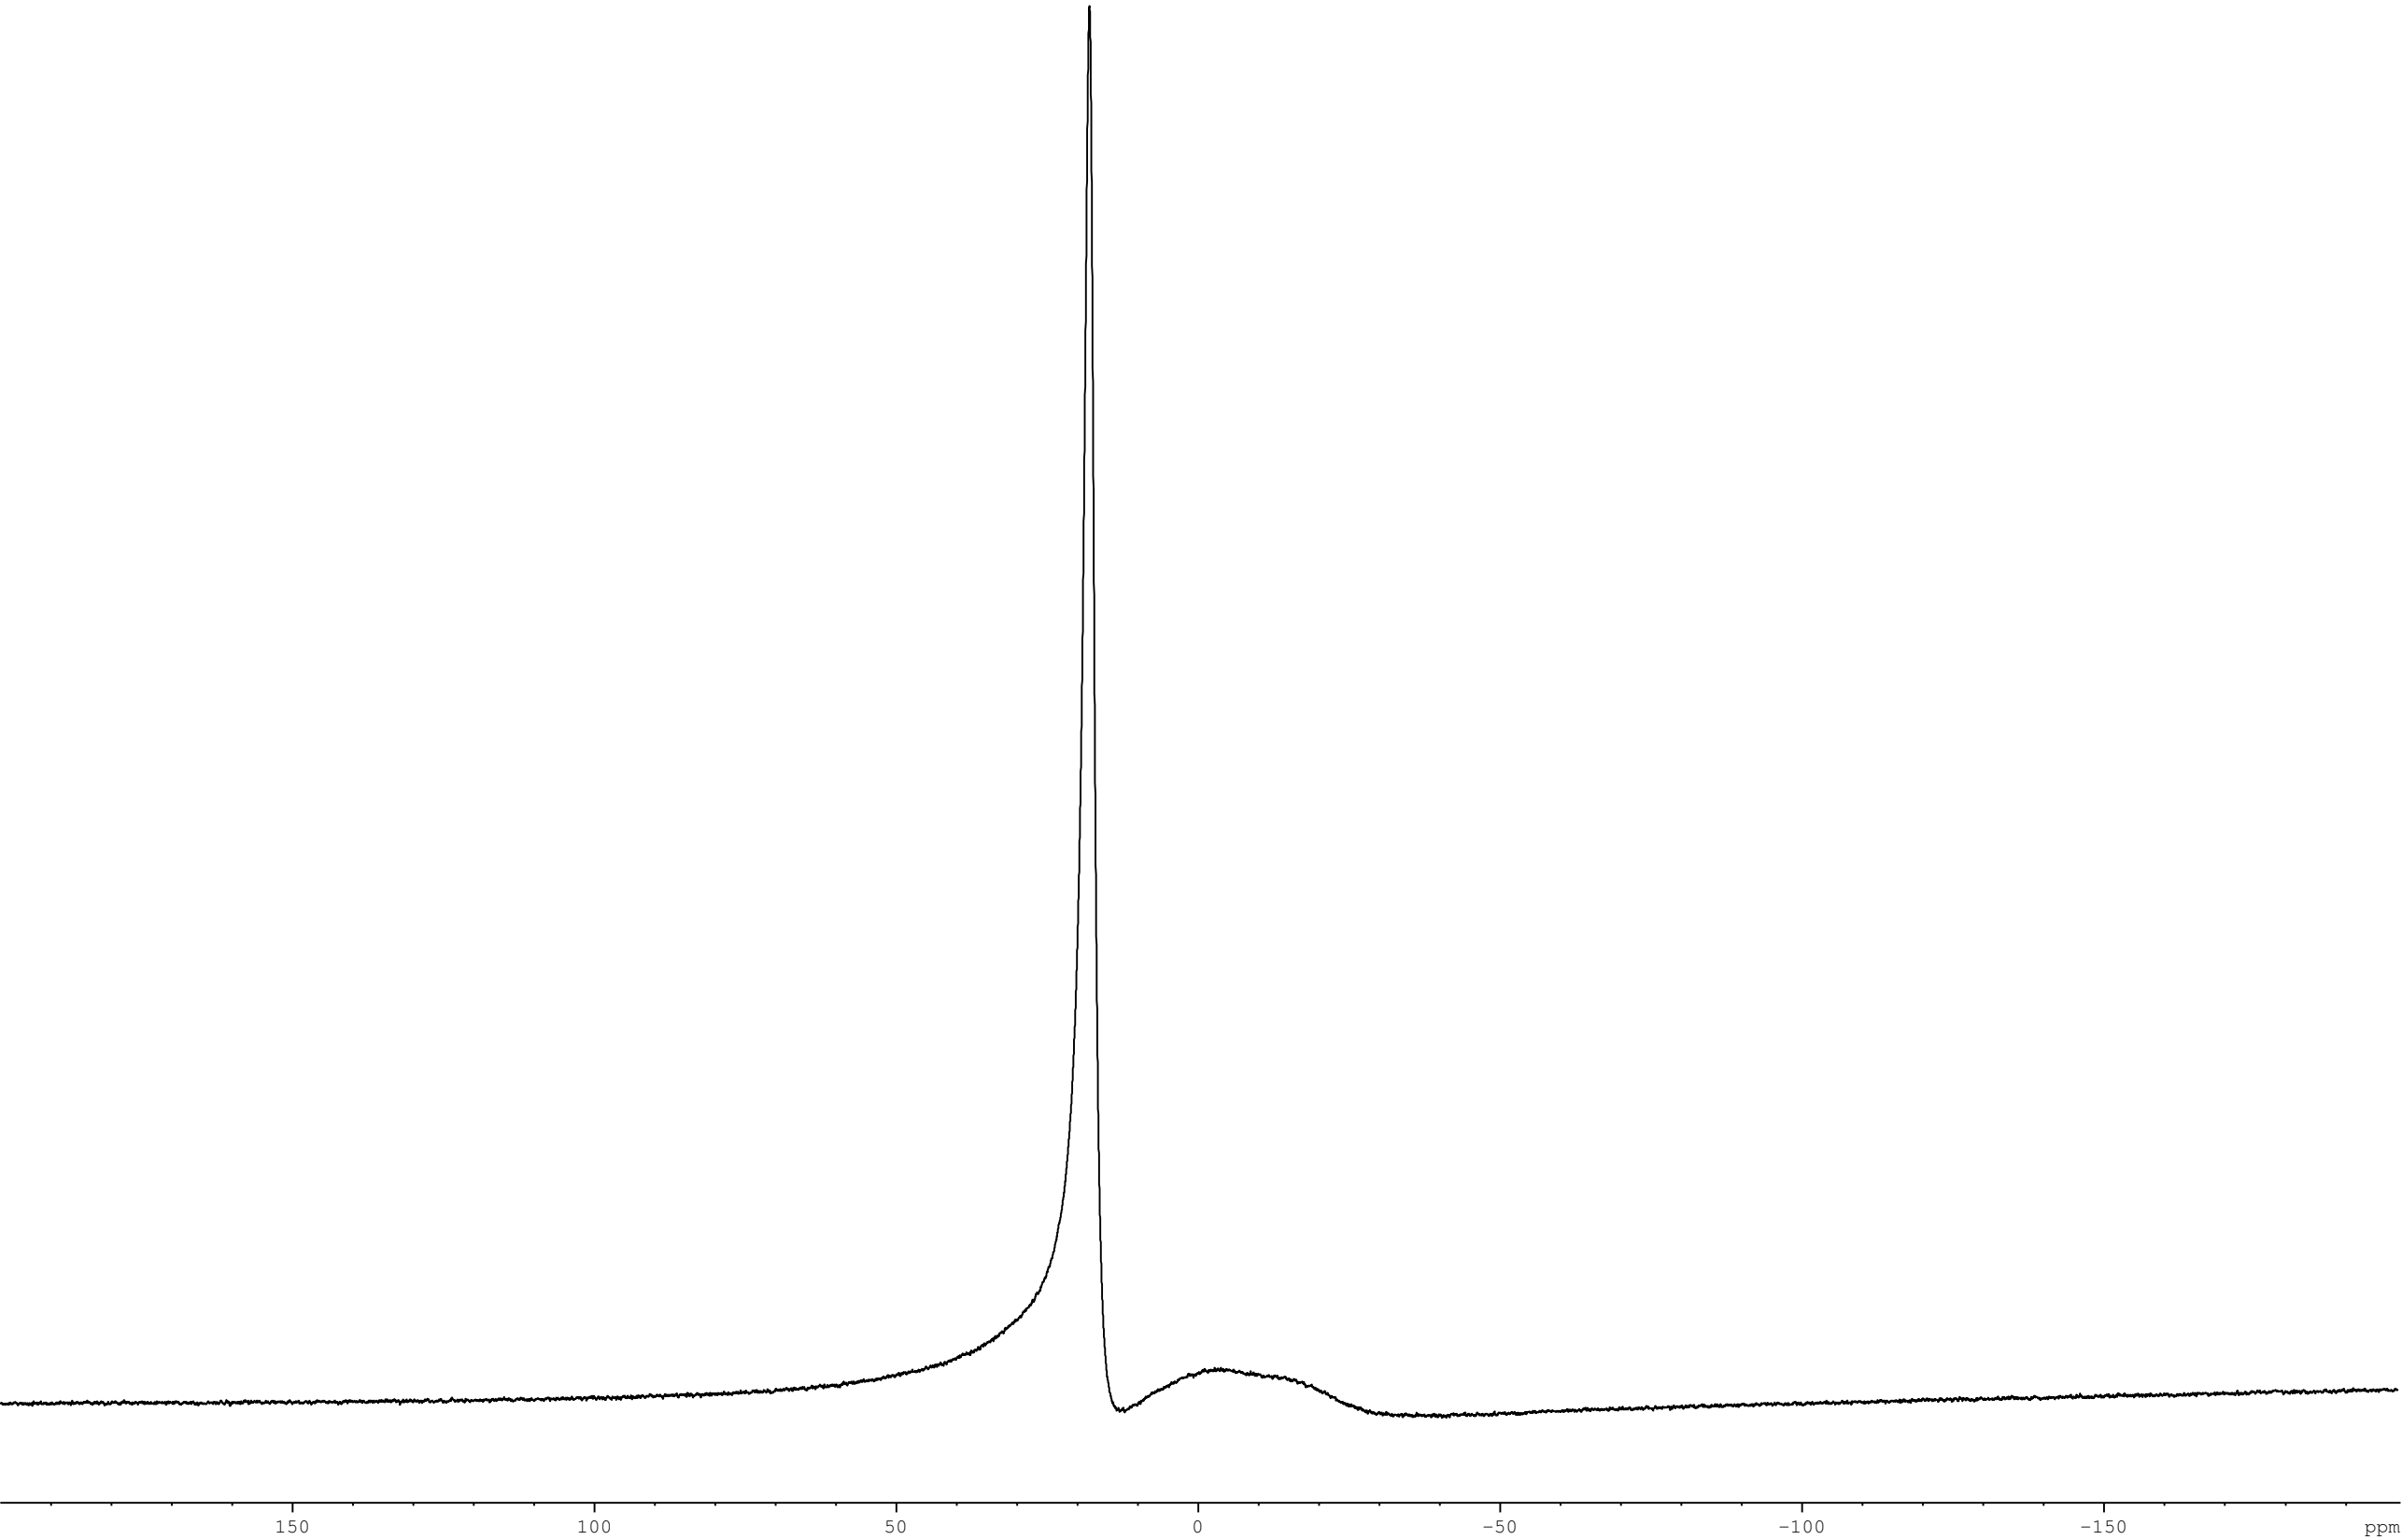

Current Data Parameters  
NAME RP107  
EXPNO 11  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20210729  
Time 14.43  
INSTRUM av400  
PROBHD 5 mm PABBO BB/  
PULPROG zgbs  
TD 102034  
SOLVENT CDCl3  
NS 128  
DS 0  
SWH 51020.406 Hz  
FIDRES 0.500033 Hz  
AQ 0.9999332 s  
RG 645  
DW 9.800 us  
DE 6.50 us  
TE 298.2 K  
D1 0.30000001 s  
TD0 1

===== CHANNEL f1 =====  
SFO1 128.3679801 MHz  
NUC1 11B  
P1 15.00 us  
P2 30.00 us  
PLW1 22.00000000 W

F2 - Processing parameters  
SI 32768  
SF 128.3679800 MHz  
WDW EM  
SSB 0  
LB 10.00 Hz  
GB 0  
PC 1.40