


C13CPD.ucl CD3CN {U:400} tds 23

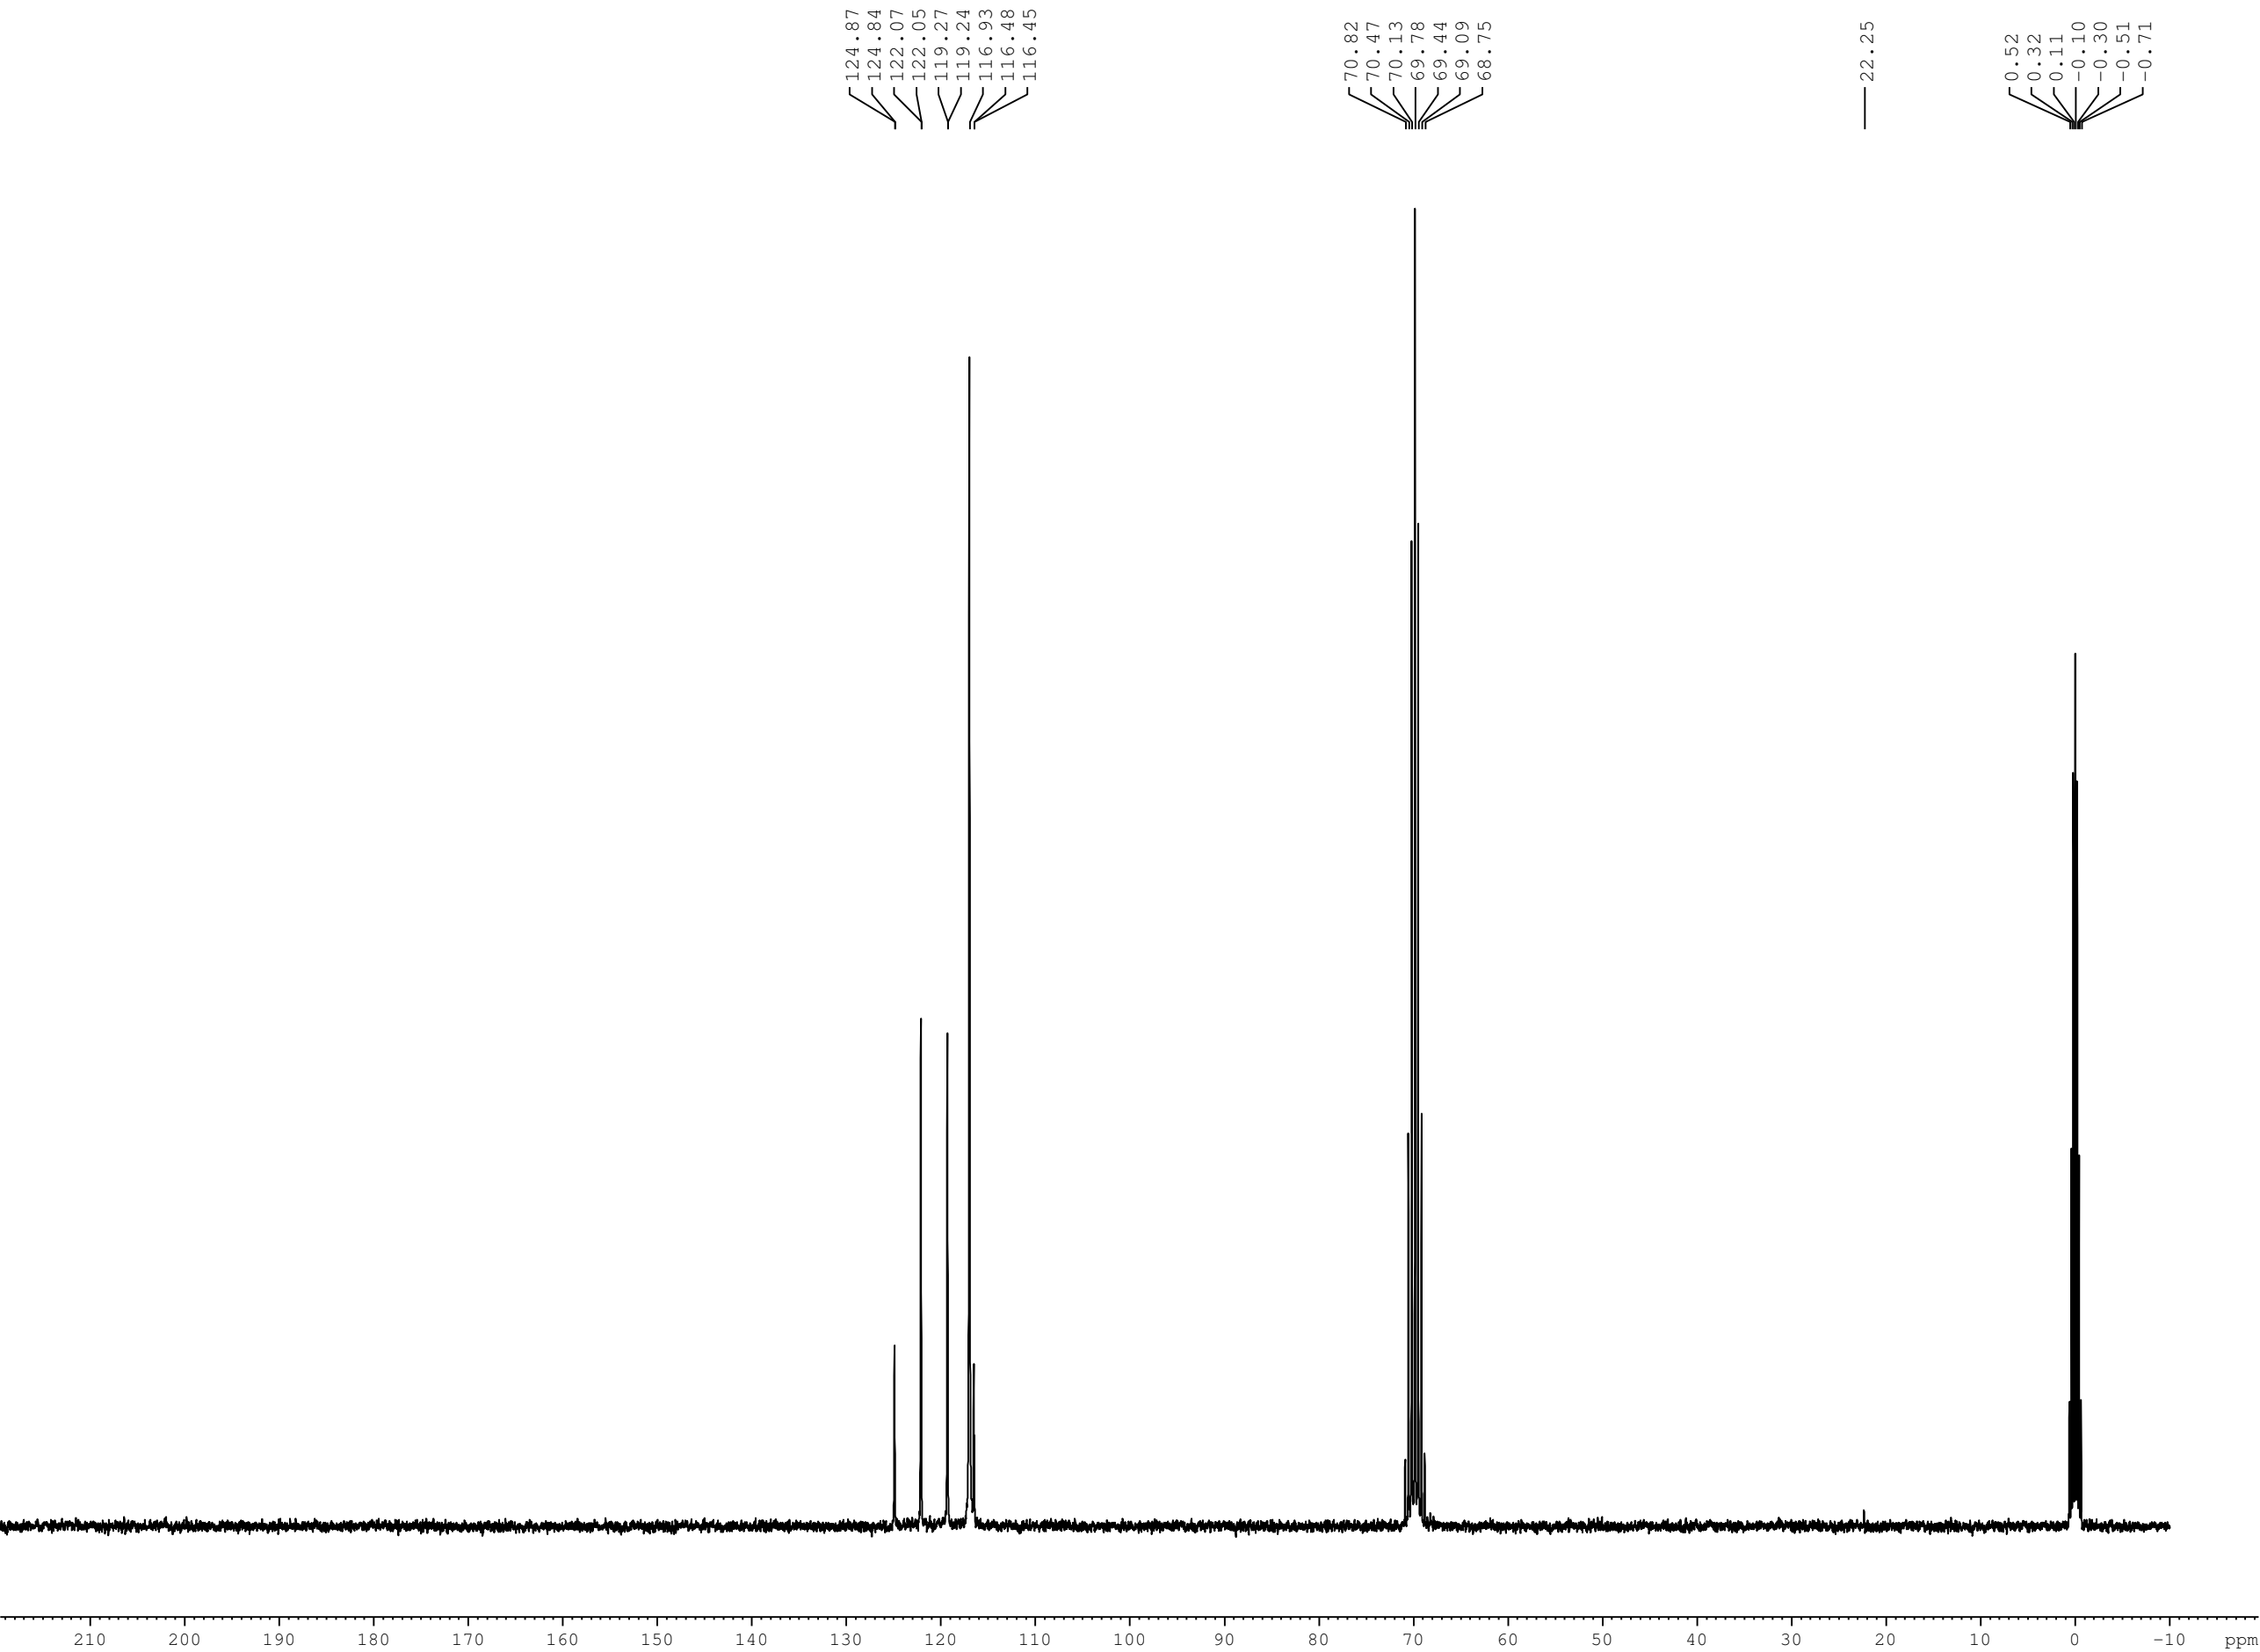

Current Data Parameters
NAME RP183 apr 24
EXPNO 14
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240409
Time 20.00
INSTRUM av400
PROBHD 5 mm PABBO BB/
PULPROG zgpg30
TD 56388
SOLVENT CD3CN
NS 128
DS 0
SWH 28195.488 Hz
FIDRES 0.500026 Hz
AQ 0.9999472 s
RG 1030
DW 17.733 µs
DE 7.15 µs
TE 296.5 K
D1 2.00000000 s
D11 0.03000000 s
TD0 8

===== CHANNEL f1 =====
SFO1 100.6183037 MHz
NUC1 13C
P1 10.00 µs
PLW1 75.00000000 W

===== CHANNEL f2 =====
SFO2 400.1016004 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 µs
PLW2 20.00000000 W
PLW12 0.48394999 W
PLW13 0.39199999 W

F2 - Processing parameters
SI 65536
SF 100.6052250 MHz
WDW EM
SSB 0
LB 2.00 Hz
GB 0
PC 1.40