


F19CPD.ucl CD3CN {U:\400} tds 23

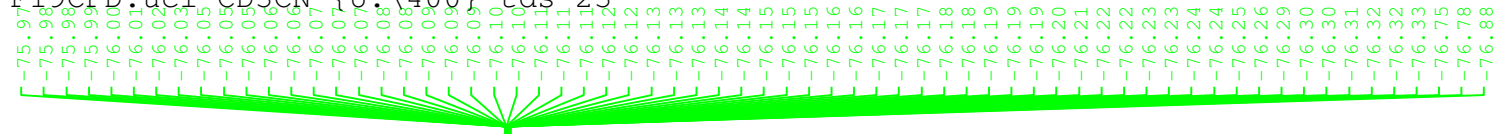


Current Data Parameters  
NAME RP183 apr 24  
EXPNO 13  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20240409  
Time 16.19  
INSTRUM av400  
PROBHD 5 mm PABBO BB/  
PULPROG zgfhigqn.2  
TD 131072  
SOLVENT CD3CN  
NS 16  
DS 4  
SWH 98684.211 Hz  
FIDRES 0.752901 Hz  
AQ 0.6640981 sec  
RG 90.5  
DW 5.067 usec  
DE 6.50 usec  
TE 294.3 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
D12 0.00002000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 376.4249616 MHz  
NUC1 19F  
P1 11.60 usec  
PLW1 26.00000000 W

===== CHANNEL f2 =====  
SFO2 400.1016004 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 20.00000000 W  
PLW12 0.48394999 W

F2 - Processing parameters  
SI 131072  
SF 376.4701380 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

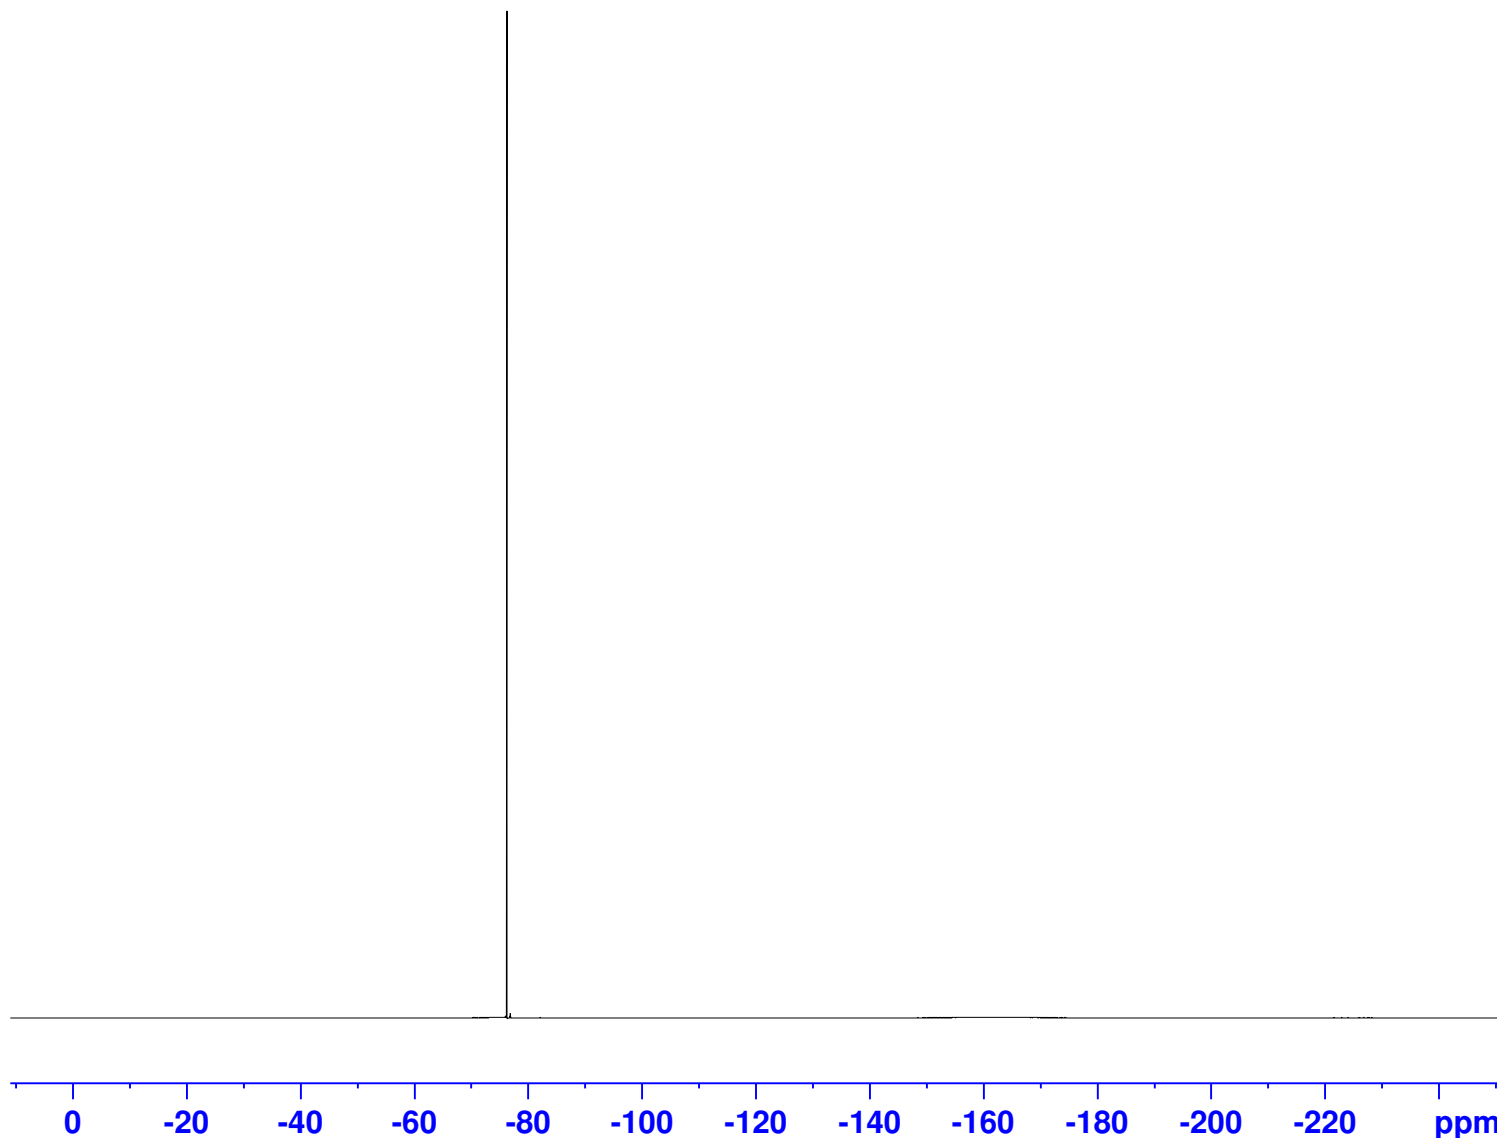

5.78  
0.35

3.58

0.99