
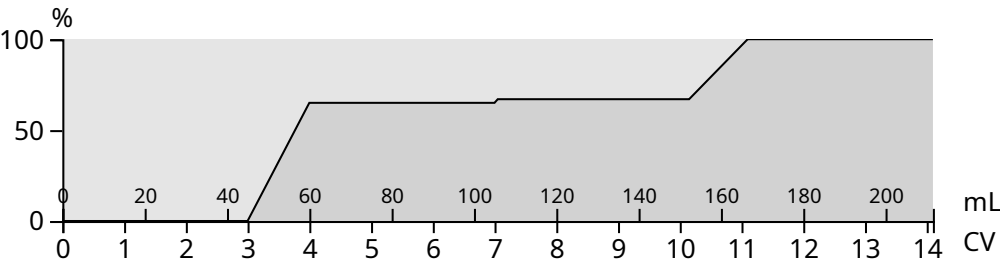


HI-2-74

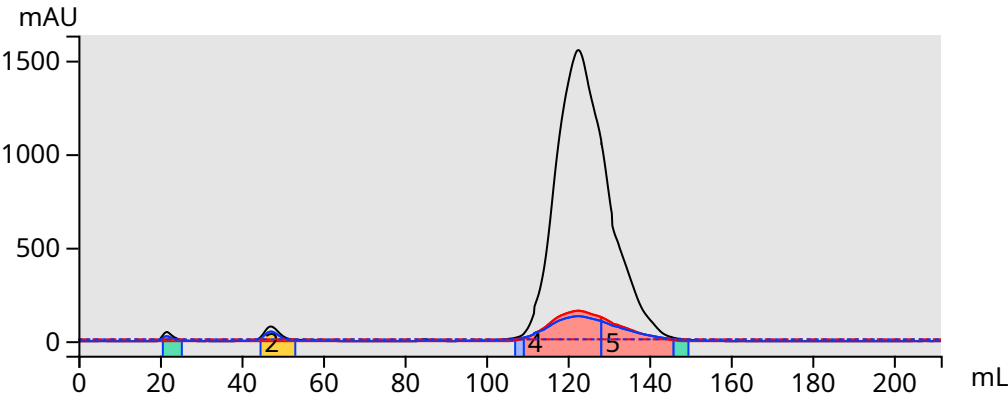

Signal	Wavelength	Threshold
● λ -All	200 - 400 nm	
● UV1 (Collect)	254 nm	10 mAU
● UV2 (Collect)	280 nm	10 mAU

Gradient

Solvent A: n-Hexane

Solvent B: Ethyl acetate

0-0%	Ethyl acetate in n-Hexane	3 CV	
0-65%	Ethyl acetate in n-Hexane	1 CV	
65-65%	Ethyl acetate in n-Hexane	3 CV	
65-67%	Ethyl acetate in n-Hexane	0.1 CV	
67-67%	Ethyl acetate in n-Hexane	3.1 CV	Isocratic hold
67-100%	Ethyl acetate in n-Hexane	0.9 CV	
100-100%	Ethyl acetate in n-Hexane	3 CV	

Run Parameters

Column Type: Biotage® Sfär 10g

Flow Rate: 40 mL/min

Equilibration: On

Collect All: Off


Channel: 1

Sample Mass: 150

Max Fraction Volume: 19 mL

UV Baseline Correction: On

Racks

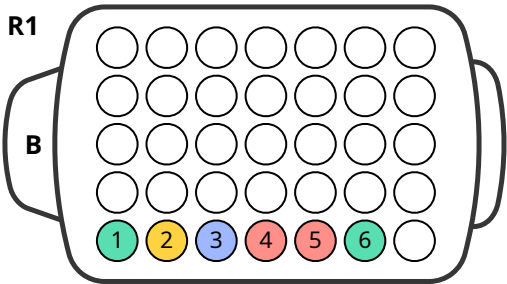

Rack Type: 16 x 150 mm, 19 mL

Rack ID: 16142028410799003245

System Information

Software: SELEKT 1.3.2-11737

Instrument ID: AAA-BCJ-INN-EPH

Log

Message	Run Phase	Volume	Time
Run started by user.	Not Started	0 mL	16:50:19
Isocratic hold false -> true.	Gradient	106 mL	16:56:32
Isocratic hold true -> false.	Gradient	152 mL	16:57:45
Gradient changed.	Gradient	152 mL	16:57:45
Run finished.	Finished	211 mL	17:00:20