


OLS2-154 r  
OLS2-154 r 7 (0.171)

21-Dec-2023  
1: TOF MS ES+  
2.74e4



OLS2-154 r  
OLS2-154 r 7 (0.171)

21-Dec-2023  
1: TOF MS ES+  
6.09e3

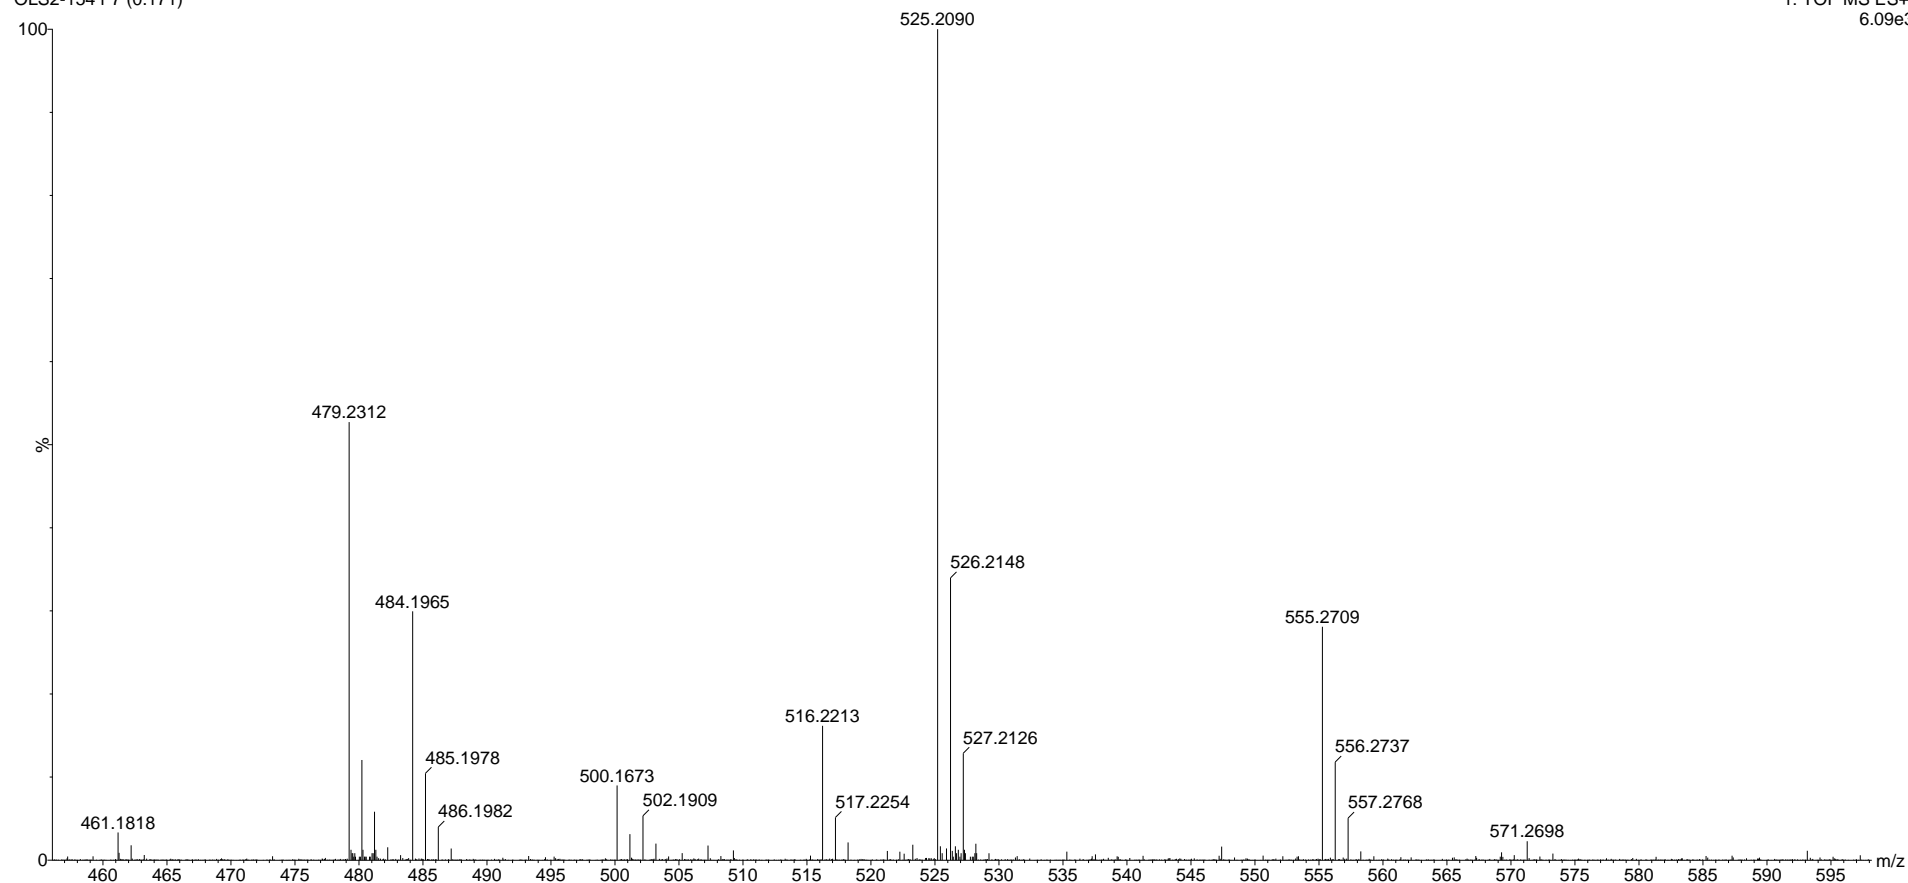

### Elemental Composition Report for 484m/z

#### Single Mass Analysis

Tolerance = 5.0 PPM / DBE: min = -1.5, max = 100.0

Element prediction: Off

Number of isotope peaks used for i-FIT = 3

Monoisotopic Mass, Even Electron Ions

312 formula(e) evaluated with 1 results within limits (all results (up to 1000) for each mass)

Elements Used:

C: 15-30   H: 0-80   N: 0-8   O: 1-8   Na: 1-1   Si: 1-1   S: 1-1

Minimum: -1.5

Maximum: 5.0   5.0   100.0

Mass	Calc. Mass	mDa	PPM	DBE	i-FIT	i-FIT (Norm)	Formula
484.1965	484.1954	1.1	2.3	8.5	84.3	0.0	C24 H35 N O4 Na Si S [M+Na]+