


B11.ucl CDCI3 {U:\400} tds 13

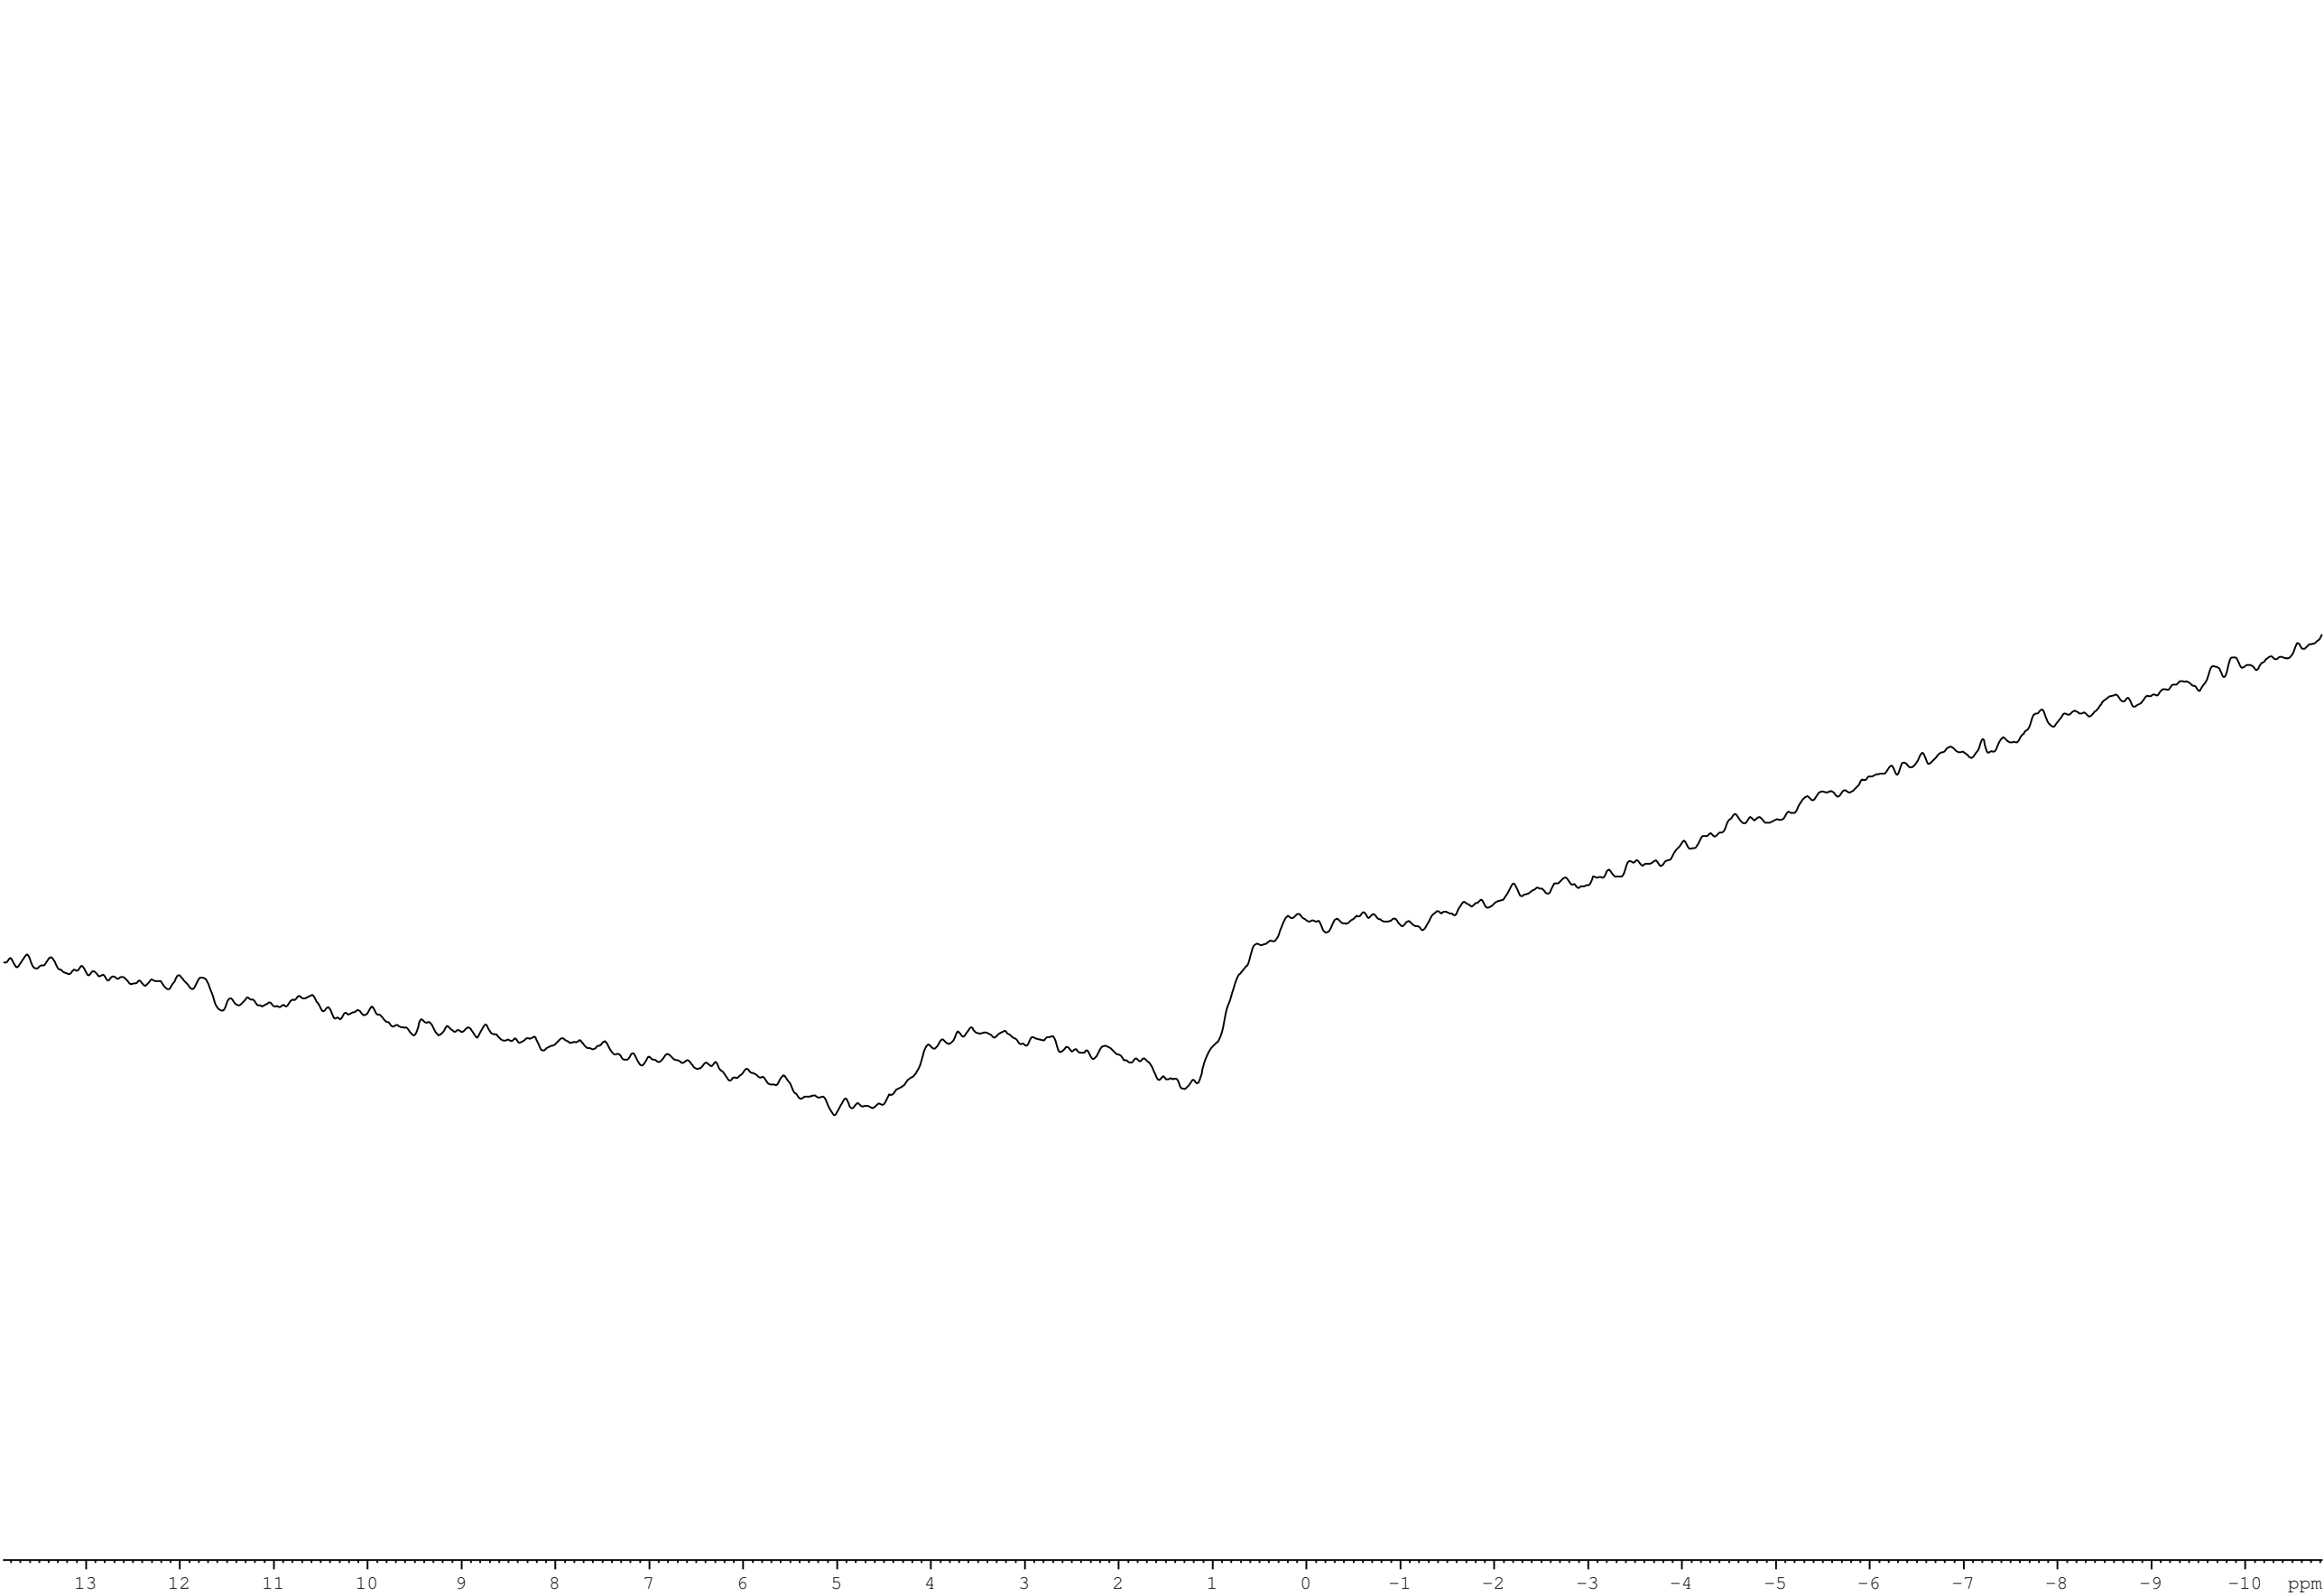

Current Data Parameters  
NAME RP457 weekend  
EXPNO 11  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20240206  
Time 14.58  
INSTRUM av400  
PROBHD 5 mm PABBO BB/  
PULPROG zg  
TD 102034  
SOLVENT CDCl3  
NS 64  
DS 0  
SWH 51020.406 Hz  
FIDRES 0.500033 Hz  
AQ 0.9999332 s  
RG 724  
DW 9.800 μs  
DE 6.50 μs  
TE 294.0 K  
D1 1.00000000 s  
TD0 1

===== CHANNEL f1 =====  
SFO1 128.3673381 MHz  
NUC1 13B  
P1 15.00 μs  
PLW1 22.00000000 W

F2 - Processing parameters  
SI 32768  
SF 128.3679800 MHz  
WDW EM  
SSB 0  
LB 10.00 Hz  
GB 0  
PC 1.00