


SL906 column

Av-400C

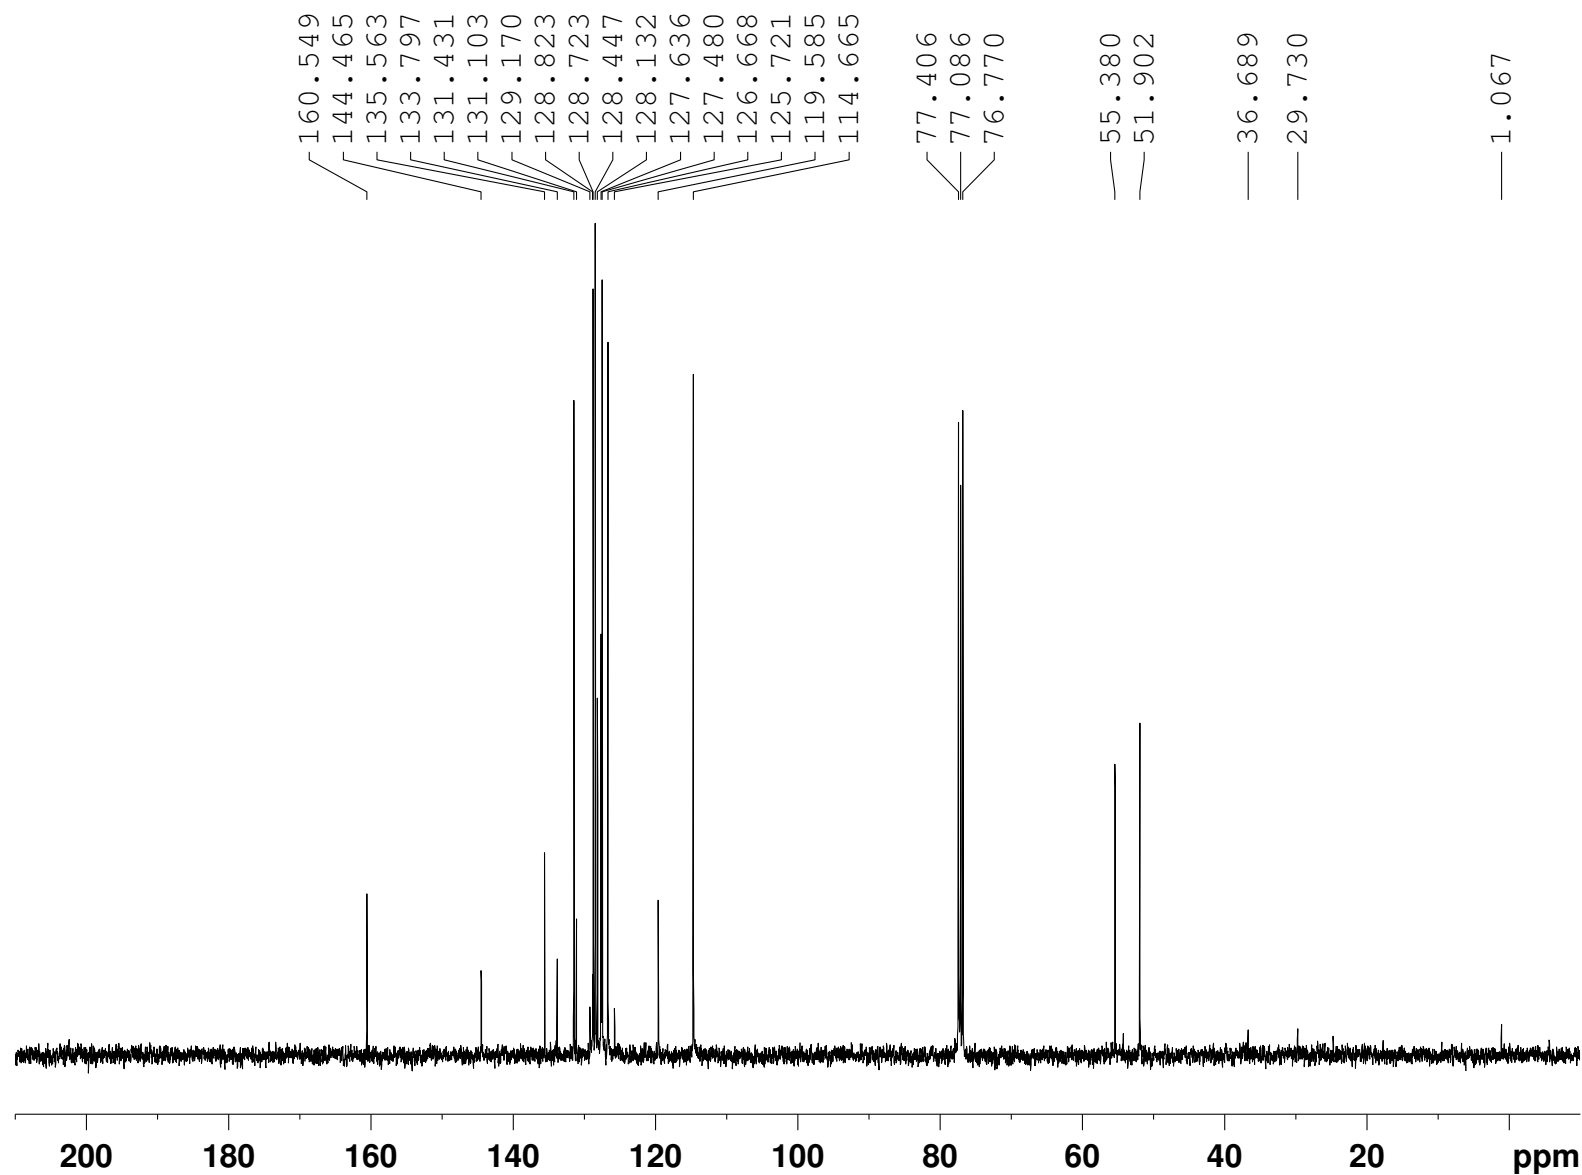

NAME Jan29-2013
EXPNO 21
PROCNO 1
Date_ 20130130
Time 1.36
INSTRUM spect
PROBHD 5 mm PABBO BB-
PULPROG zgpg30
TD 32768
SOLVENT CDCl3
NS 296
DS 4
SWH 28409.092 Hz
FIDRES 0.866977 Hz
AQ 0.5767668 sec
RG 2050
DW 17.600 usec
DE 20.00 usec
TE 296.0 K
D1 1.00000000 sec
D11 0.03000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 13C
P1 7.90 usec
PL1 -3.00 dB
PL1W 69.16384125 W
SFO1 100.6414393 MHz

===== CHANNEL f2 =====
CPDPRG2 waltz16
NUC2 1H
PCPD2 100.00 usec
PL2 -3.00 dB
PL12 16.25 dB
PL13 17.00 dB
PL2W 15.63704205 W
PL12W 0.18584658 W
PL13W 0.15637042 W
SFO2 400.2020010 MHz
SI 16384
SF 100.6303700 MHz
WDW EM
SSB 0
LB 2.00 Hz
GB 0
PC 1.40