


# A4

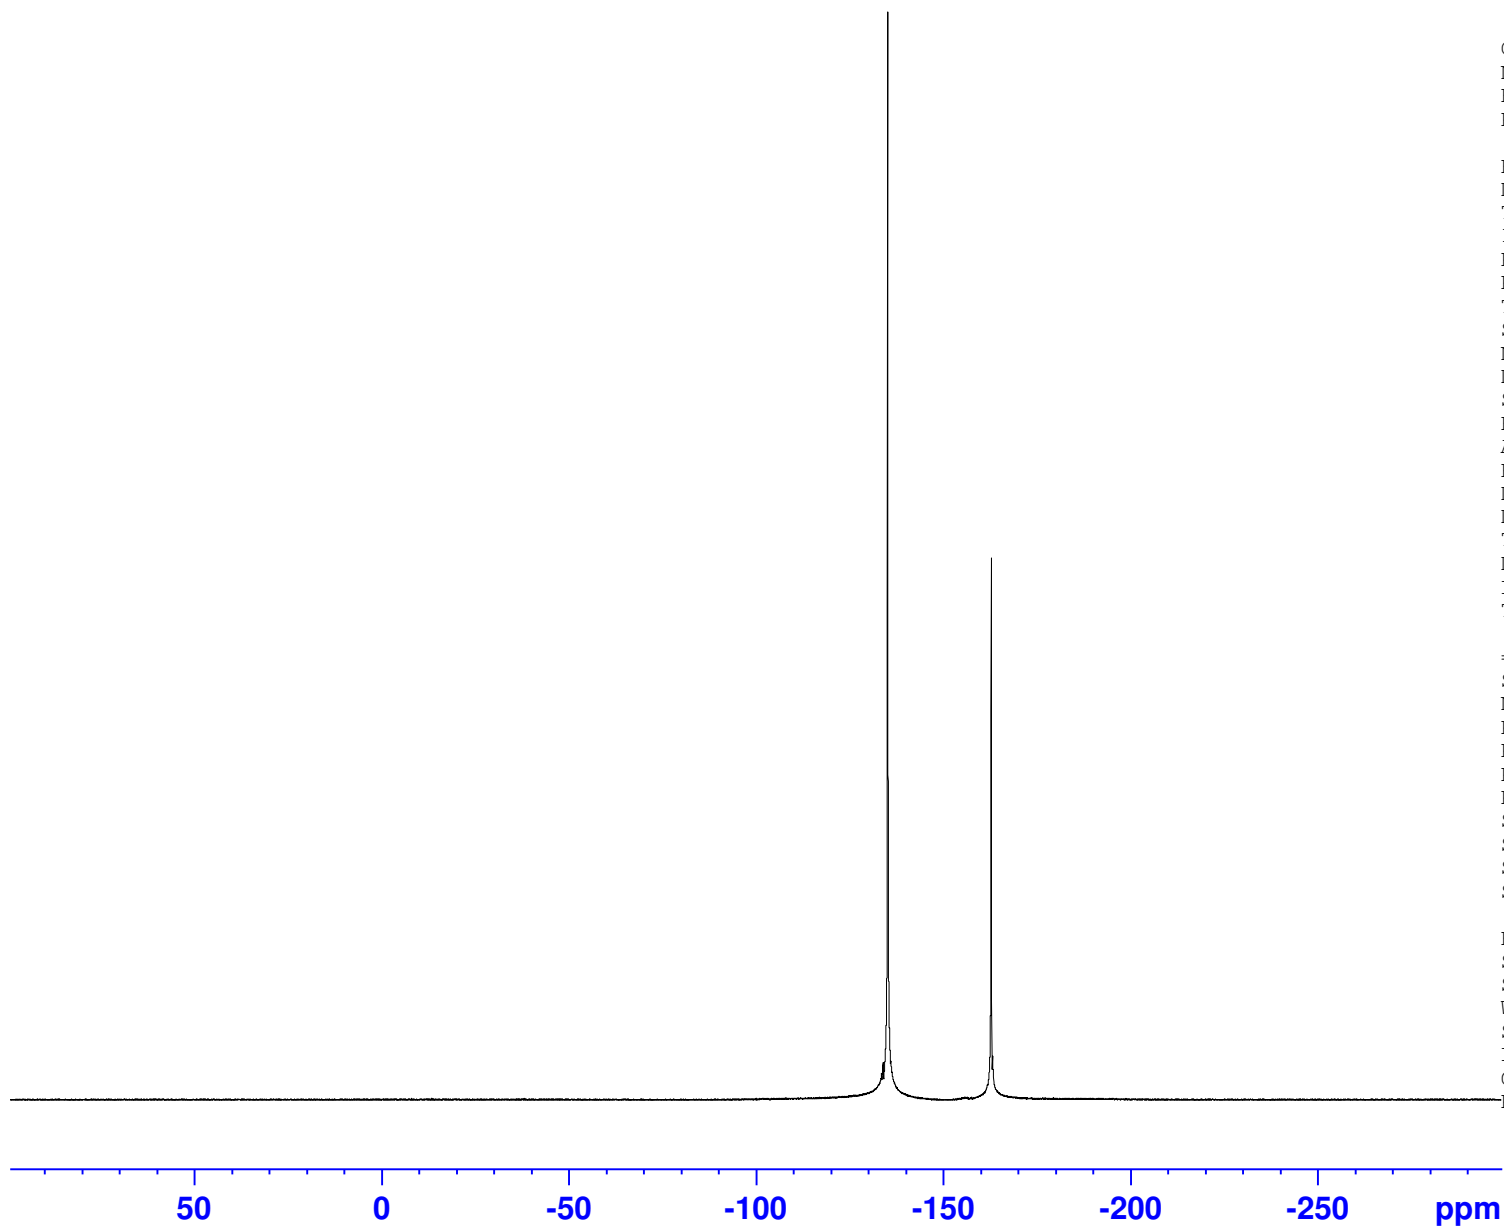

Current Data Parameters  
NAME 27170706  
EXPNO 12  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20141227  
Time 17.15  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgflqn180.b  
TD 262144  
SOLVENT CDCl3  
NS 8  
DS 0  
SWH 150000.000 Hz  
FIDRES 0.572205 Hz  
AQ 0.8738133 sec  
RG 197.36  
DW 3.333 usec  
DE 20.28 usec  
TE 294.7 K  
D1 1.00000000 sec  
L0 1  
TD0 1

===== CHANNEL f1 =====  
SFO1 376.4607164 MHz  
NUC1 19F  
P1 12.00 usec  
P26 3000.00 usec  
PLW0 0 W  
PLW1 28.00000000 W  
SPNAM[8] Crp180,3,20.2  
SPOAL8 0  
SPOFFS8 0 Hz  
SPW8 3.08019996 W

F2 - Processing parameters  
SI 262144  
SF 376.4983660 MHz  
WDW EM  
SSB 0  
LB 5.00 Hz  
GB 0  
PC 2.00