


B4

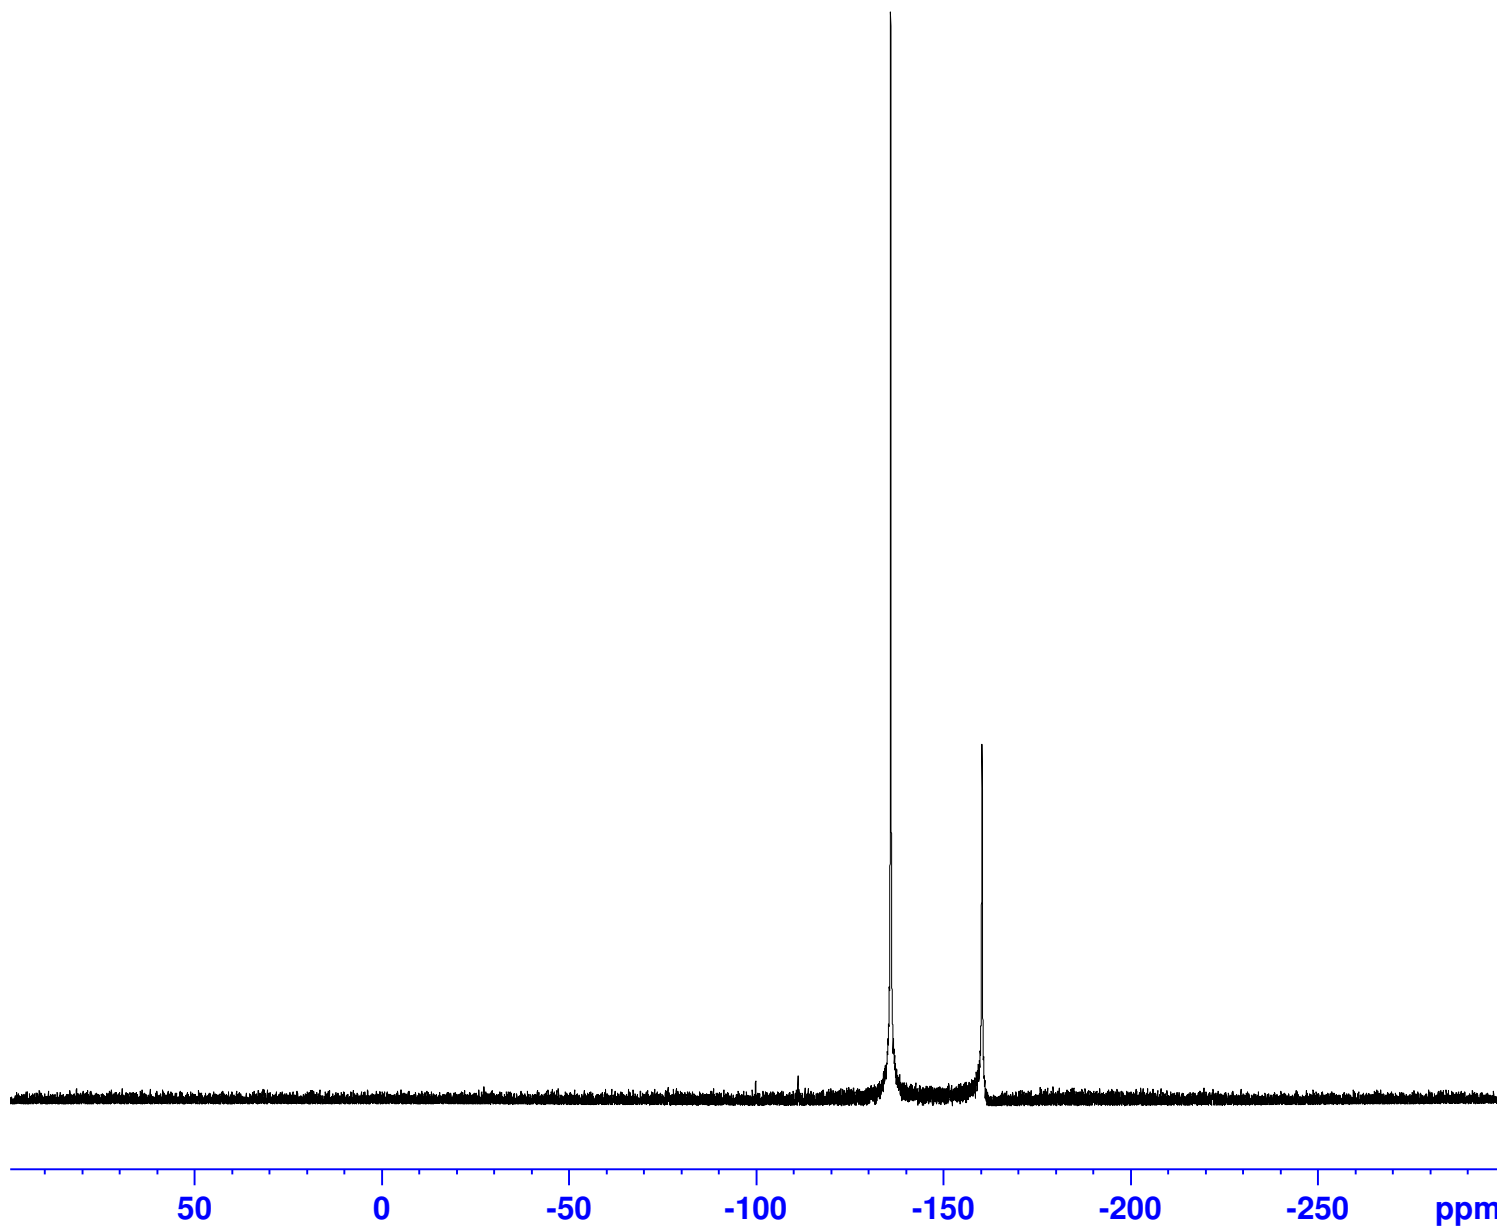

Current Data Parameters
NAME 06203545
EXPNO 12
PROCNO 1

F2 - Acquisition Parameters
Date_ 20161207
Time 6.27
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zgflqn180.b
TD 262144
SOLVENT CDCl3
NS 8
DS 0
SWH 150000.000 Hz
FIDRES 0.572205 Hz
AQ 0.8738133 sec
RG 207.78
DW 3.333 usec
DE 20.25 usec
TE 295.2 K
D1 1.00000000 sec
L0 1
TD0 1

===== CHANNEL f1 =====
SFO1 376.3976795 MHz
NUC1 19F
P1 14.00 usec
P26 3000.00 usec
PLW0 0 W
PLW1 20.00000000 W
SPNAM[8] Crp180,3,20.2
SPOAL8 0
SPOFFS8 0 Hz
SPW8 2.99469995 W

F2 - Processing parameters
SI 262144
SF 376.4353230 MHz
WDW EM
SSB 0
LB 5.00 Hz
GB 0
PC 2.00