


AW:SA:SA-165-2

# B4

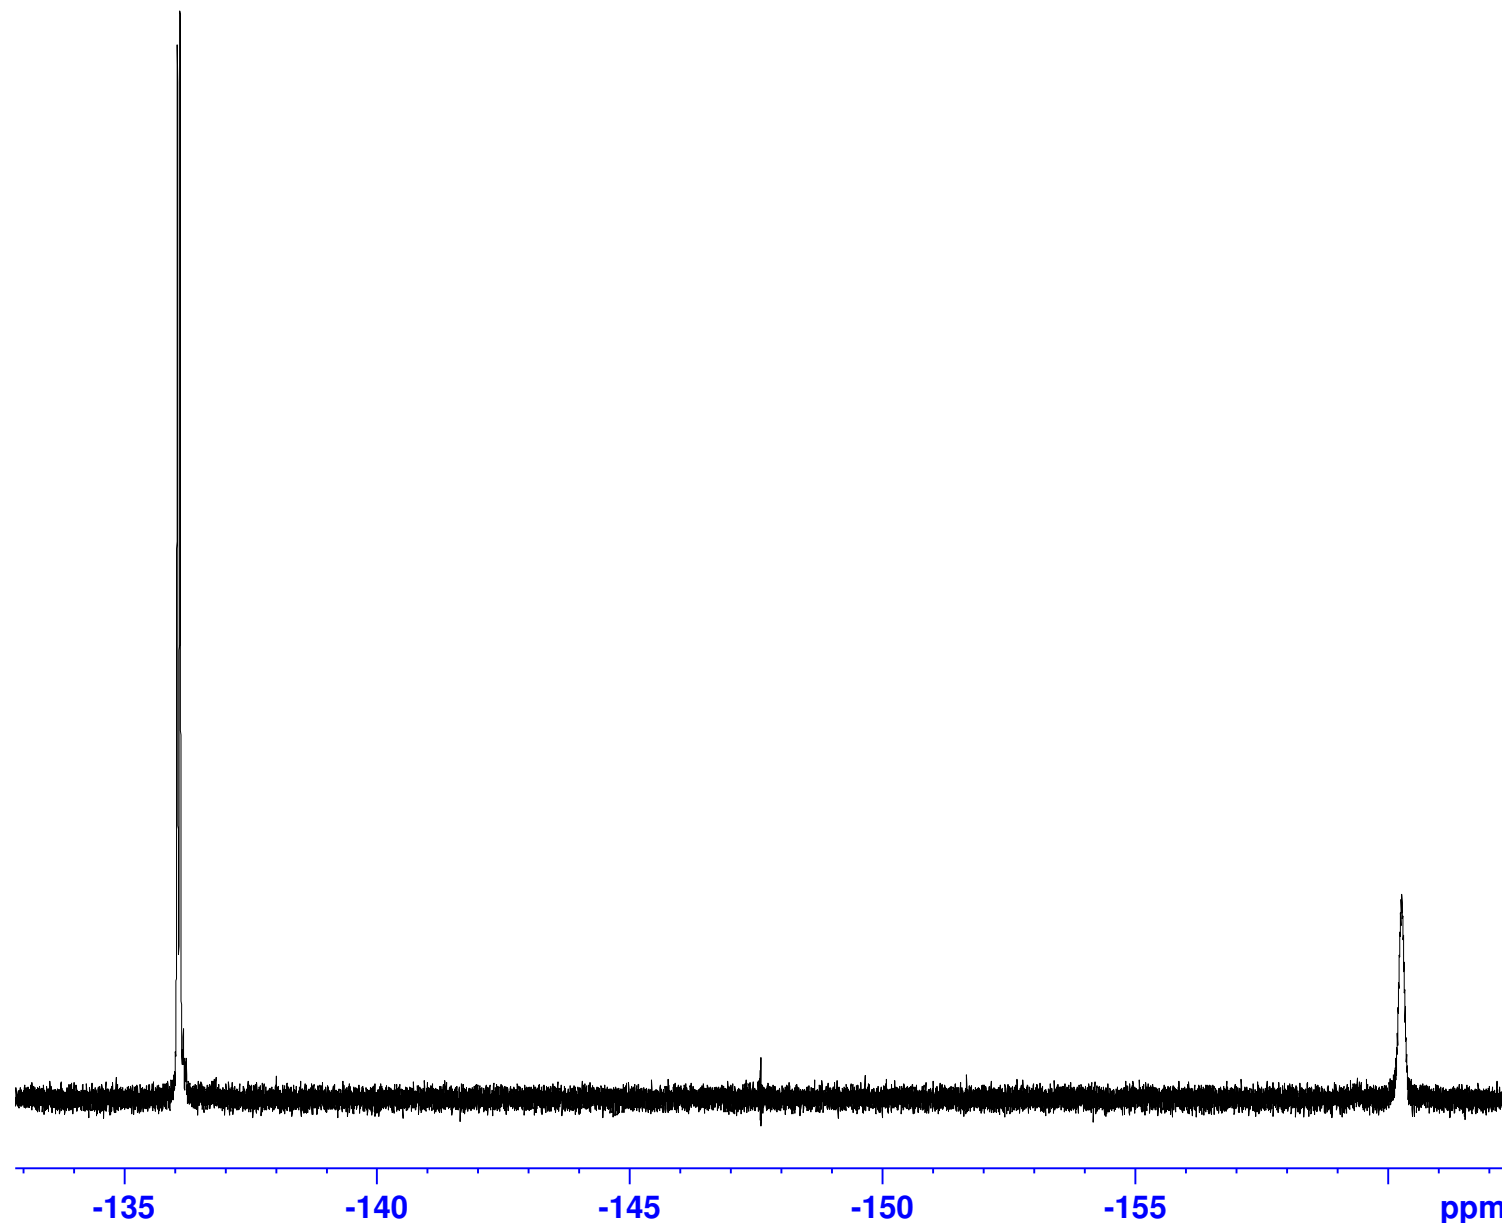

Current Data Parameters  
NAME 06203545  
EXPNO 14  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20161207  
Time 6.29  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgfhigqn180.b  
TD 39416  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 11111.111 Hz  
FIDRES 0.281893 Hz  
AQ 1.7737200 sec  
RG 207.78  
DW 45.000 usec  
DE 23.43 usec  
TE 295.9 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
D12 0.00001000 sec  
L0 1  
TD0 1

===== CHANNEL f1 =====  
SFO1 376.3797607 MHz  
NUC1 19F  
P1 14.00 usec  
P26 3000.00 usec  
PLW0 0 W  
PLW1 20.00000000 W  
SPNAM[8] Crp180,3,20.2  
SPOAL8 0  
SPOFFS8 0 Hz  
SPW8 2.99469995 W

===== CHANNEL f2 =====  
SFO2 400.0654706 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 65.00 usec  
PLW2 17.00000000 W  
PLW12 0.59887999 W

F2 - Processing parameters  
SI 262144  
SF 376.4353230 MHz  
WDW EM  
SSB 0  
LB 0.20 Hz  
GB 0  
PC 2.00