


6FS790Ax1

Av-400A

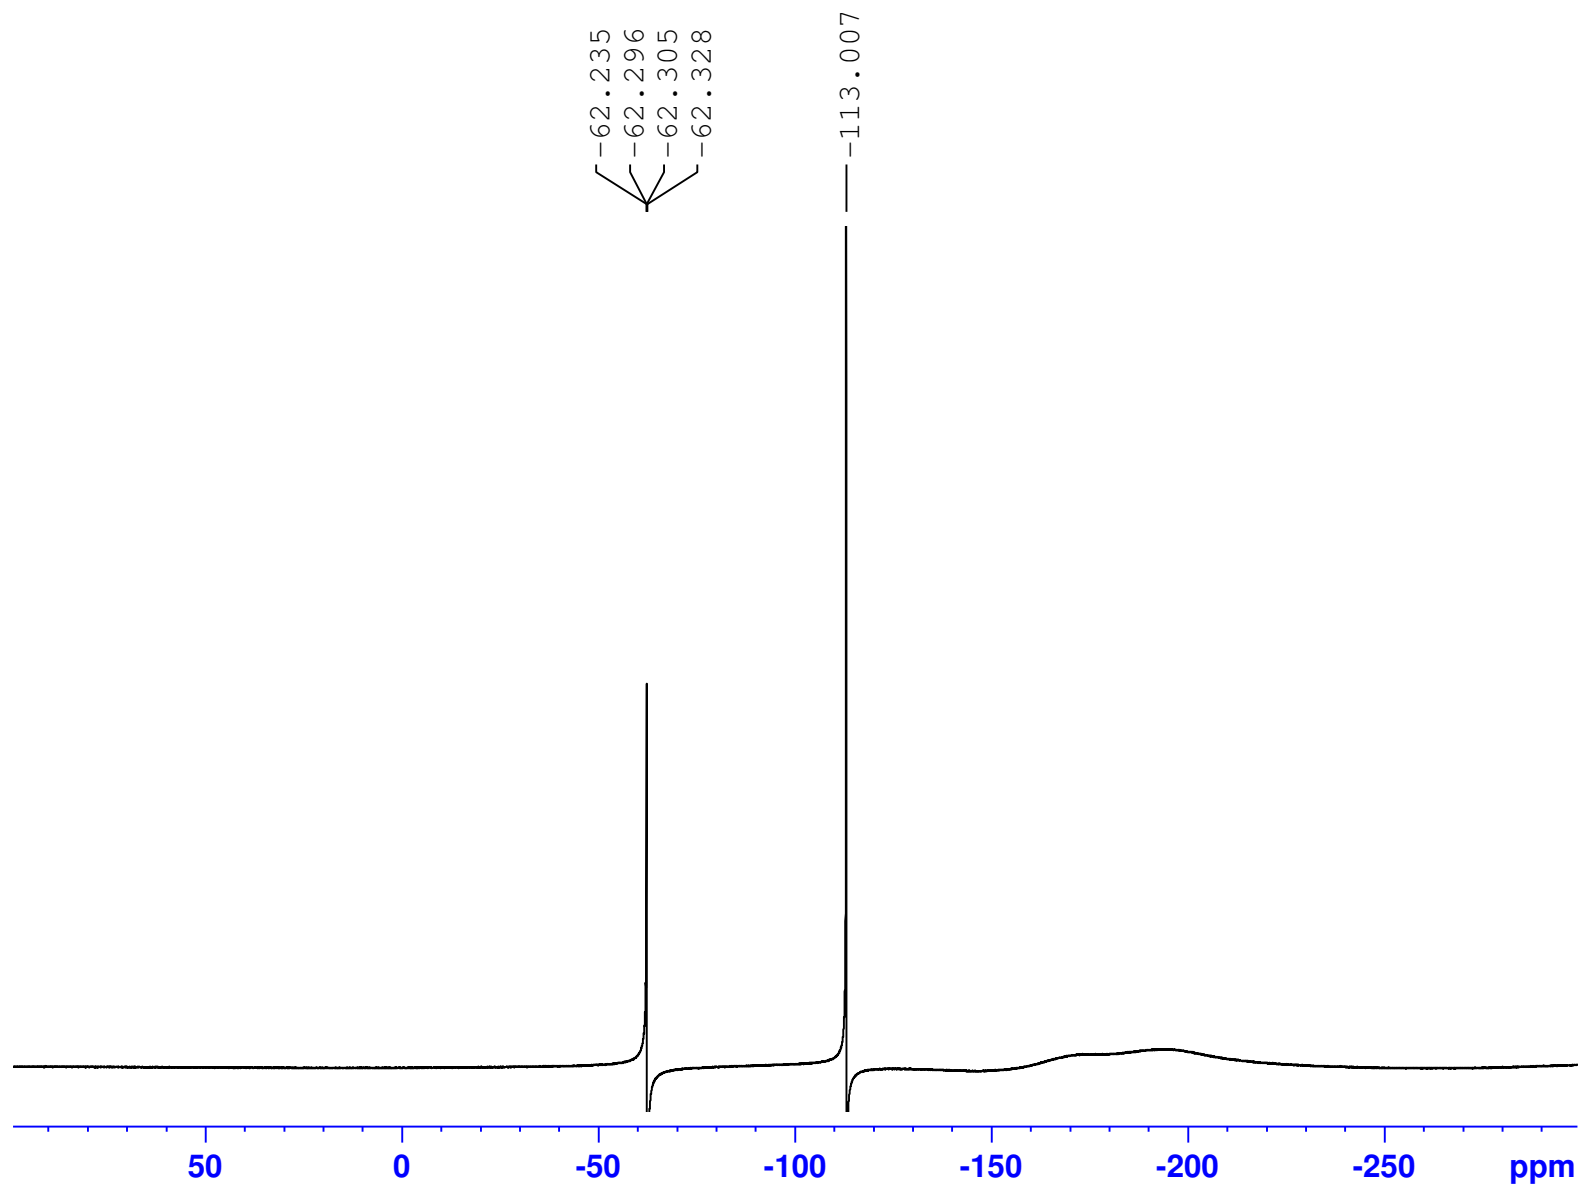

Current Data Parameters
NAME Apr07-2017
EXPNO 90
PROCNO 1

F2 - Acquisition Parameters
Date_ 20170407
Time 19.03
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zgflqn
TD 65536
SOLVENT CDCl3
NS 64
DS 4
SWH 150000.000 Hz
FIDRES 2.288818 Hz
AQ 0.2184533 sec
RG 207.33
DW 3.333 usec
DE 6.50 usec
TE 295.1 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 376.7241537 MHz
NUC1 19F
P1 14.80 usec
PLW1 19.95299911 W

F2 - Processing parameters
SI 65536
SF 376.7618290 MHz
WDW EM
SSB 0
LB 3.00 Hz
GB 0
PC 1.00