


AB5-480

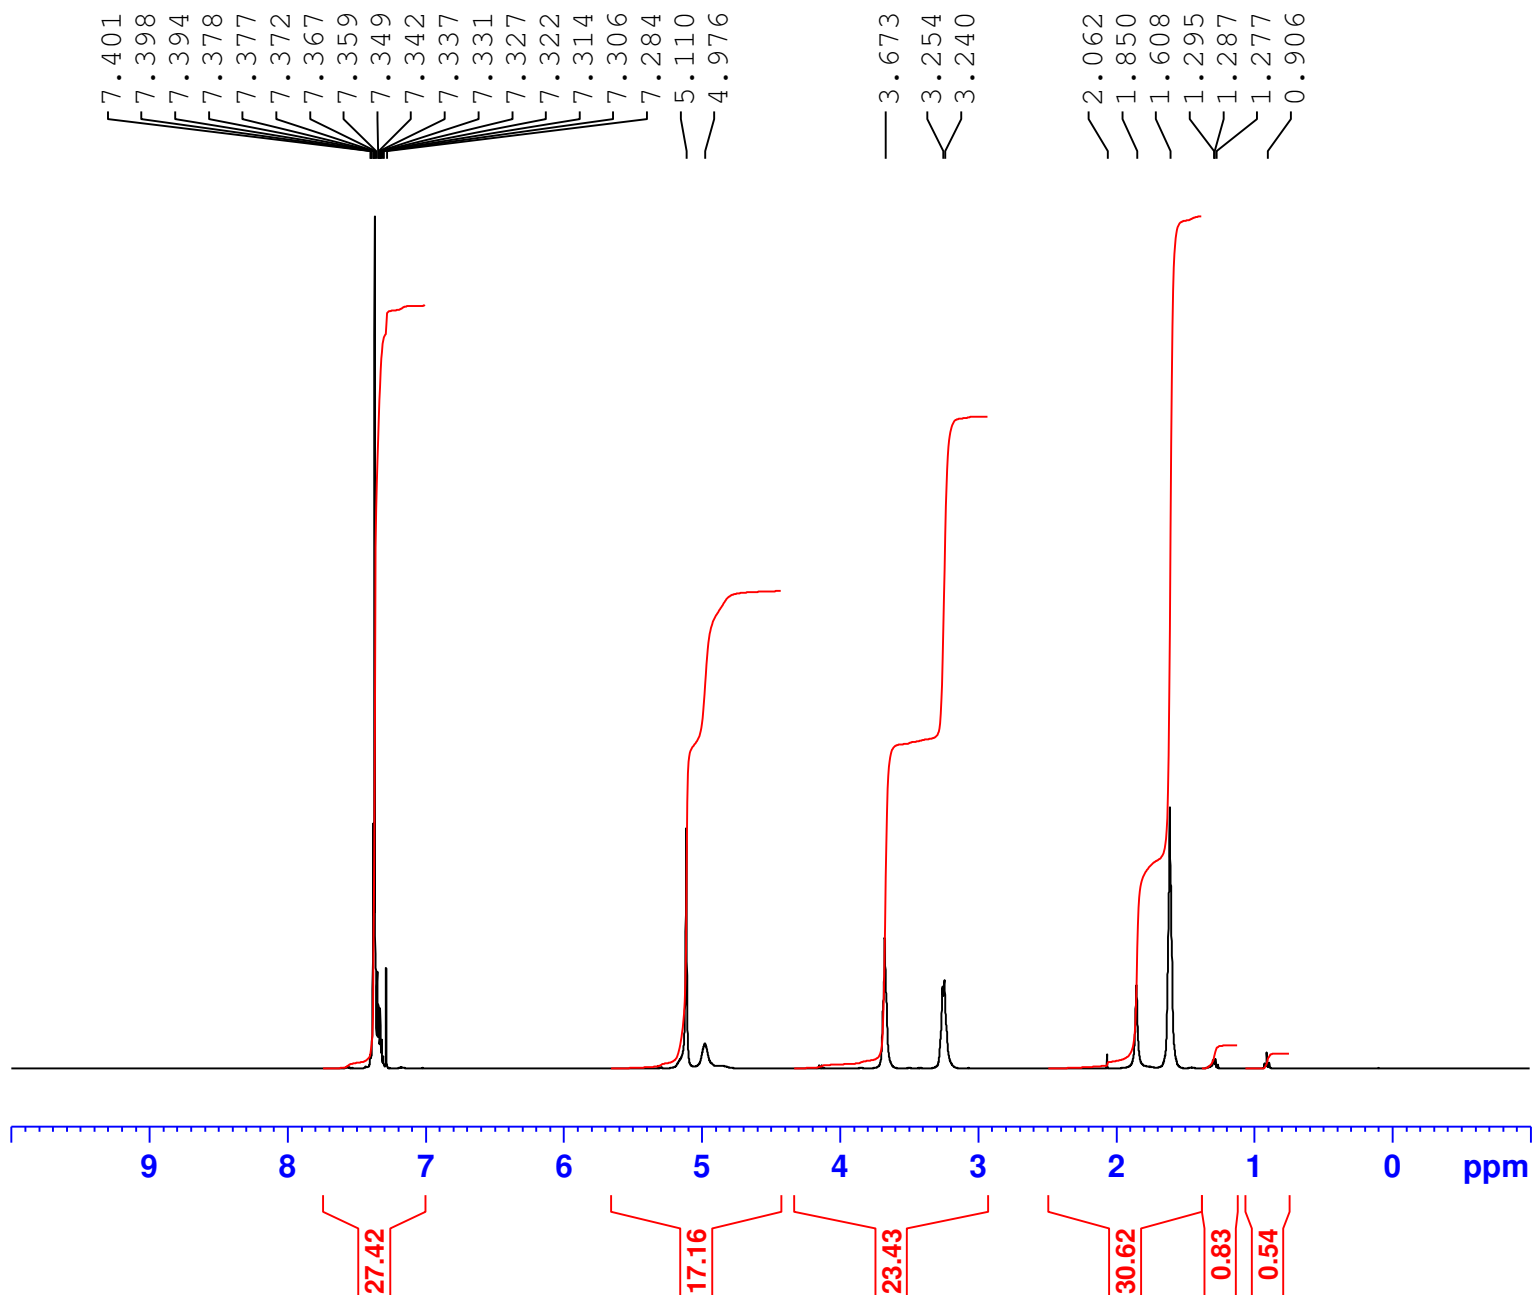

400D

Current Data Parameters
NAME Jul10-2018
EXPNO 160
PROCNO 1

F2 - Acquisition Parameters
Date_ 20180710
Time 19.18
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 32768
SOLVENT CDCl3
NS 16
DS 4
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 2.0447233 sec
RG 57.33
DW 62.400 usec
DE 6.50 usec
TE 298.3 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 400.0524003 MHz
NUC1 1H
P1 9.75 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.0500000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00