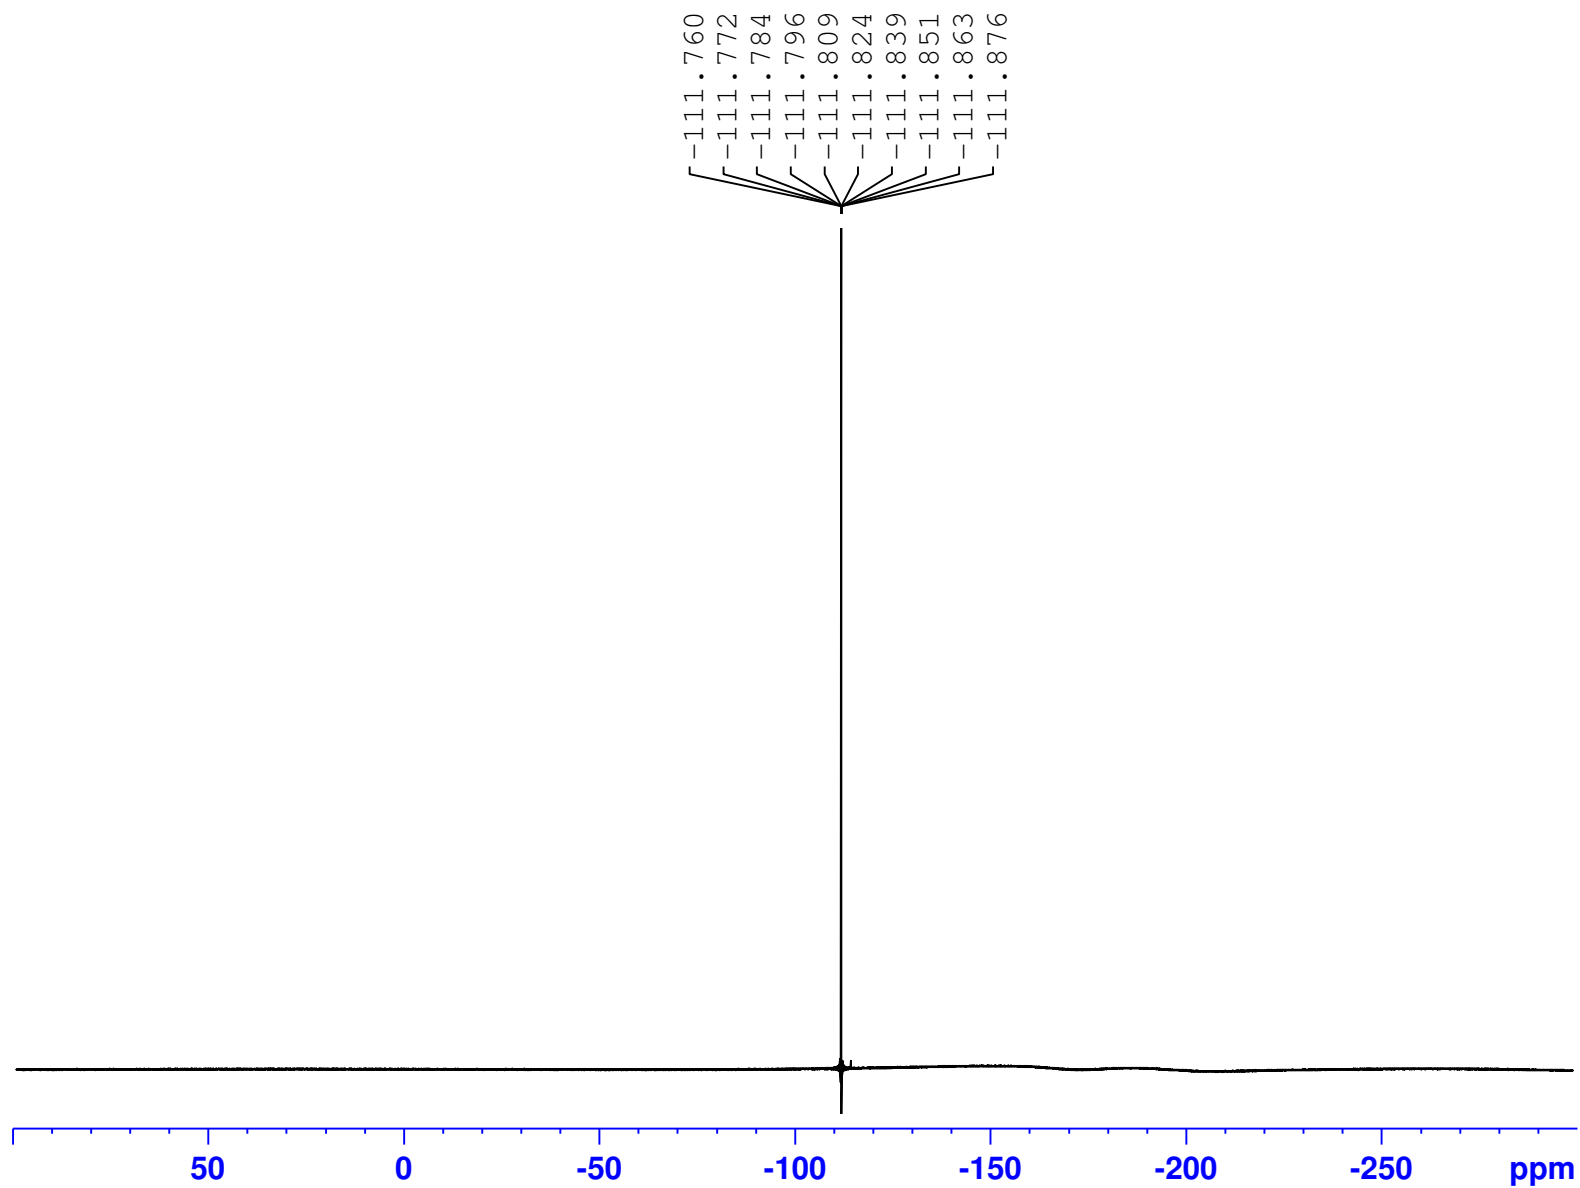


**Av-400A**

Current Data Parameters  
NAME Apr12-2018  
EXPNO 23  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20180412  
Time 19.45  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgfhigqn  
TD 65536  
SOLVENT CDCl3  
NS 64  
DS 4  
SWH 150000.000 Hz  
FIDRES 2.288818 Hz  
AQ 0.2184533 sec  
RG 207.33  
DW 3.333 usec  
DE 6.50 usec  
TE 296.3 K  
D1 1.00000000 sec  
D11 0.03000000 sec  
D12 0.00002000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 376.7241532 MHz  
NUC1 19F  
P1 14.80 usec  
PLW1 19.95299911 W

===== CHANNEL f2 =====  
SFO2 400.4119220 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 19.95299911 W  
PLW12 0.29267001 W

F2 - Processing parameters  
SI 131072  
SF 376.7618290 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.00