


SG1-020

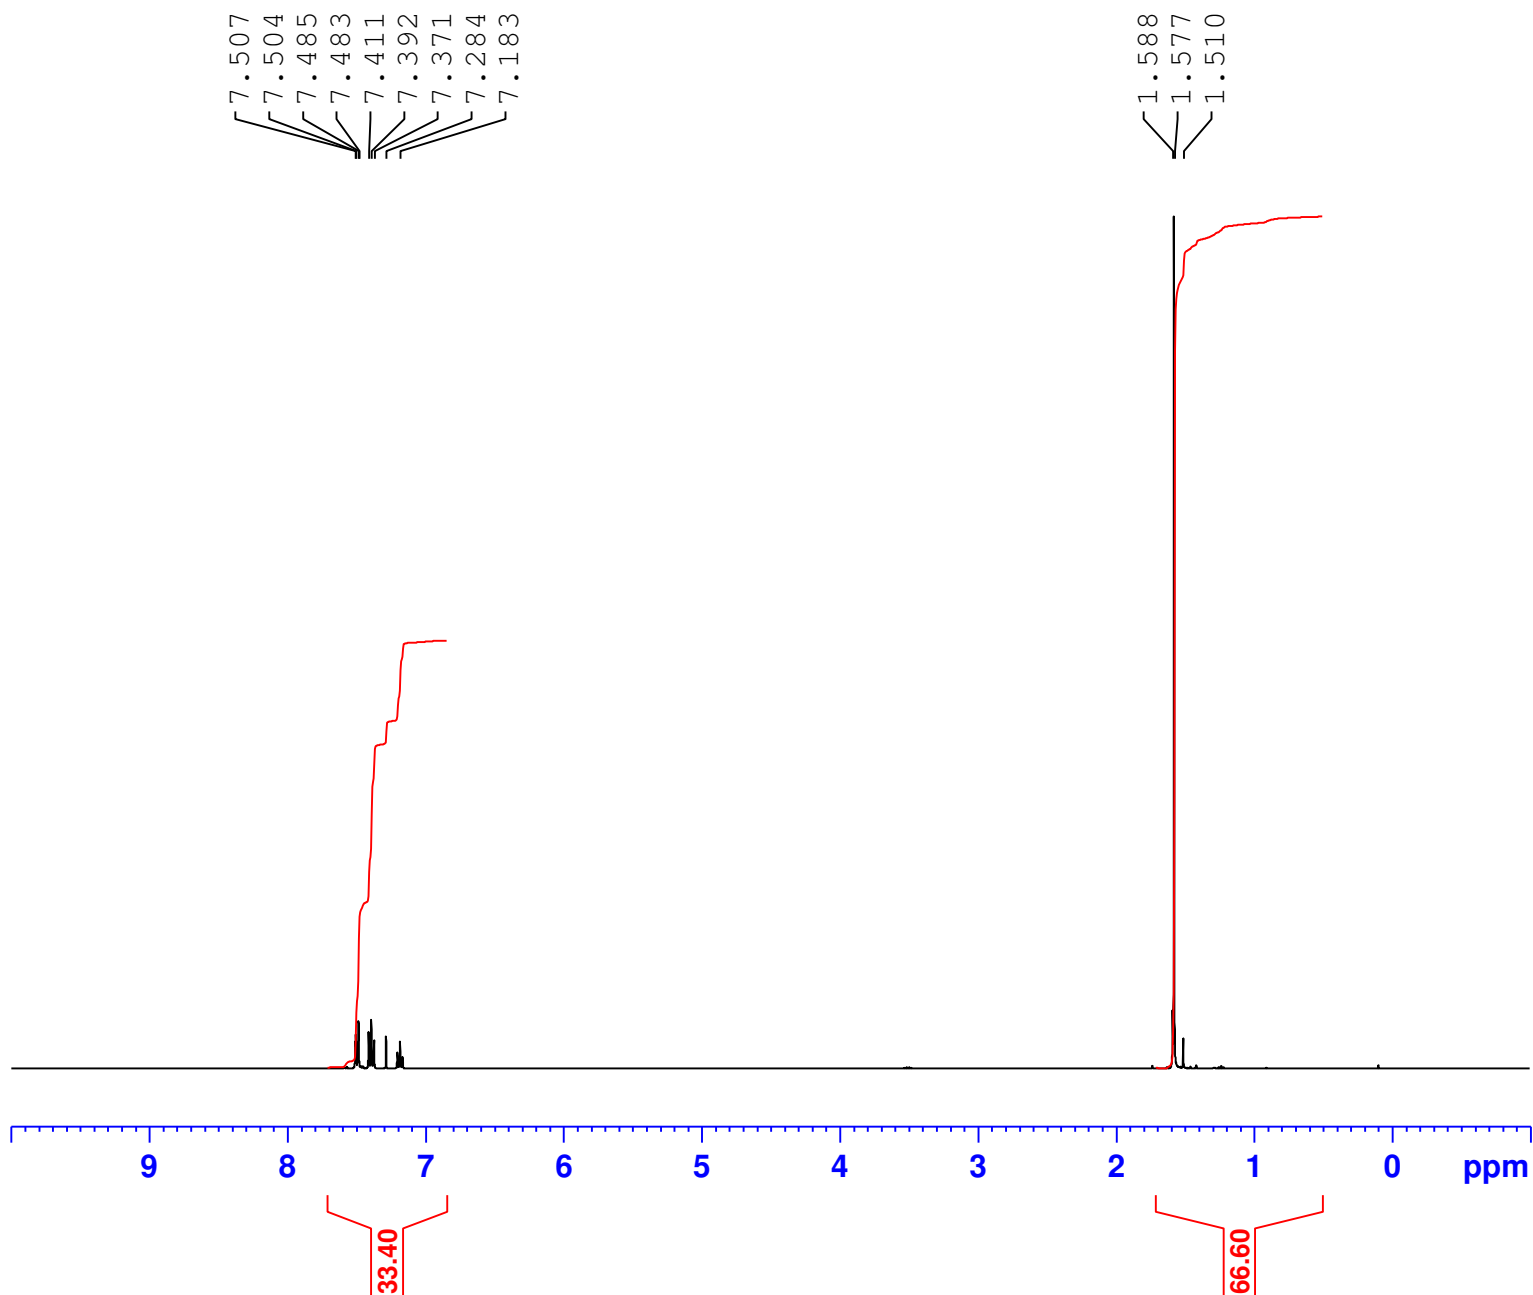

**400D**

Current Data Parameters  
NAME Jul18-2018  
EXPNO 10  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20180718  
Time 17.36  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 32768  
SOLVENT CDCl3  
NS 16  
DS 4  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 2.0447233 sec  
RG 70.87  
DW 62.400 usec  
DE 6.50 usec  
TE 296.4 K  
D1 1.00000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 400.0524003 MHz  
NUC1 1H  
P1 9.75 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.0500000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00