

Ref C10 OBz  
Group Bures\_J  
C13\_CPD\_Night1024


CDCl3 /mnt/mrdata/Bures\_J/h11997ca12

165.63  
165.38

133.81  
133.76  
133.71  
133.39  
128.54  
128.52  
128.33  
128.31

77.34  
77.22  
77.02  
76.90  
74.67  
64.72

34.21  
33.83  
31.73  
29.71  
28.60  
25.02  
22.53  
21.91  
14.00

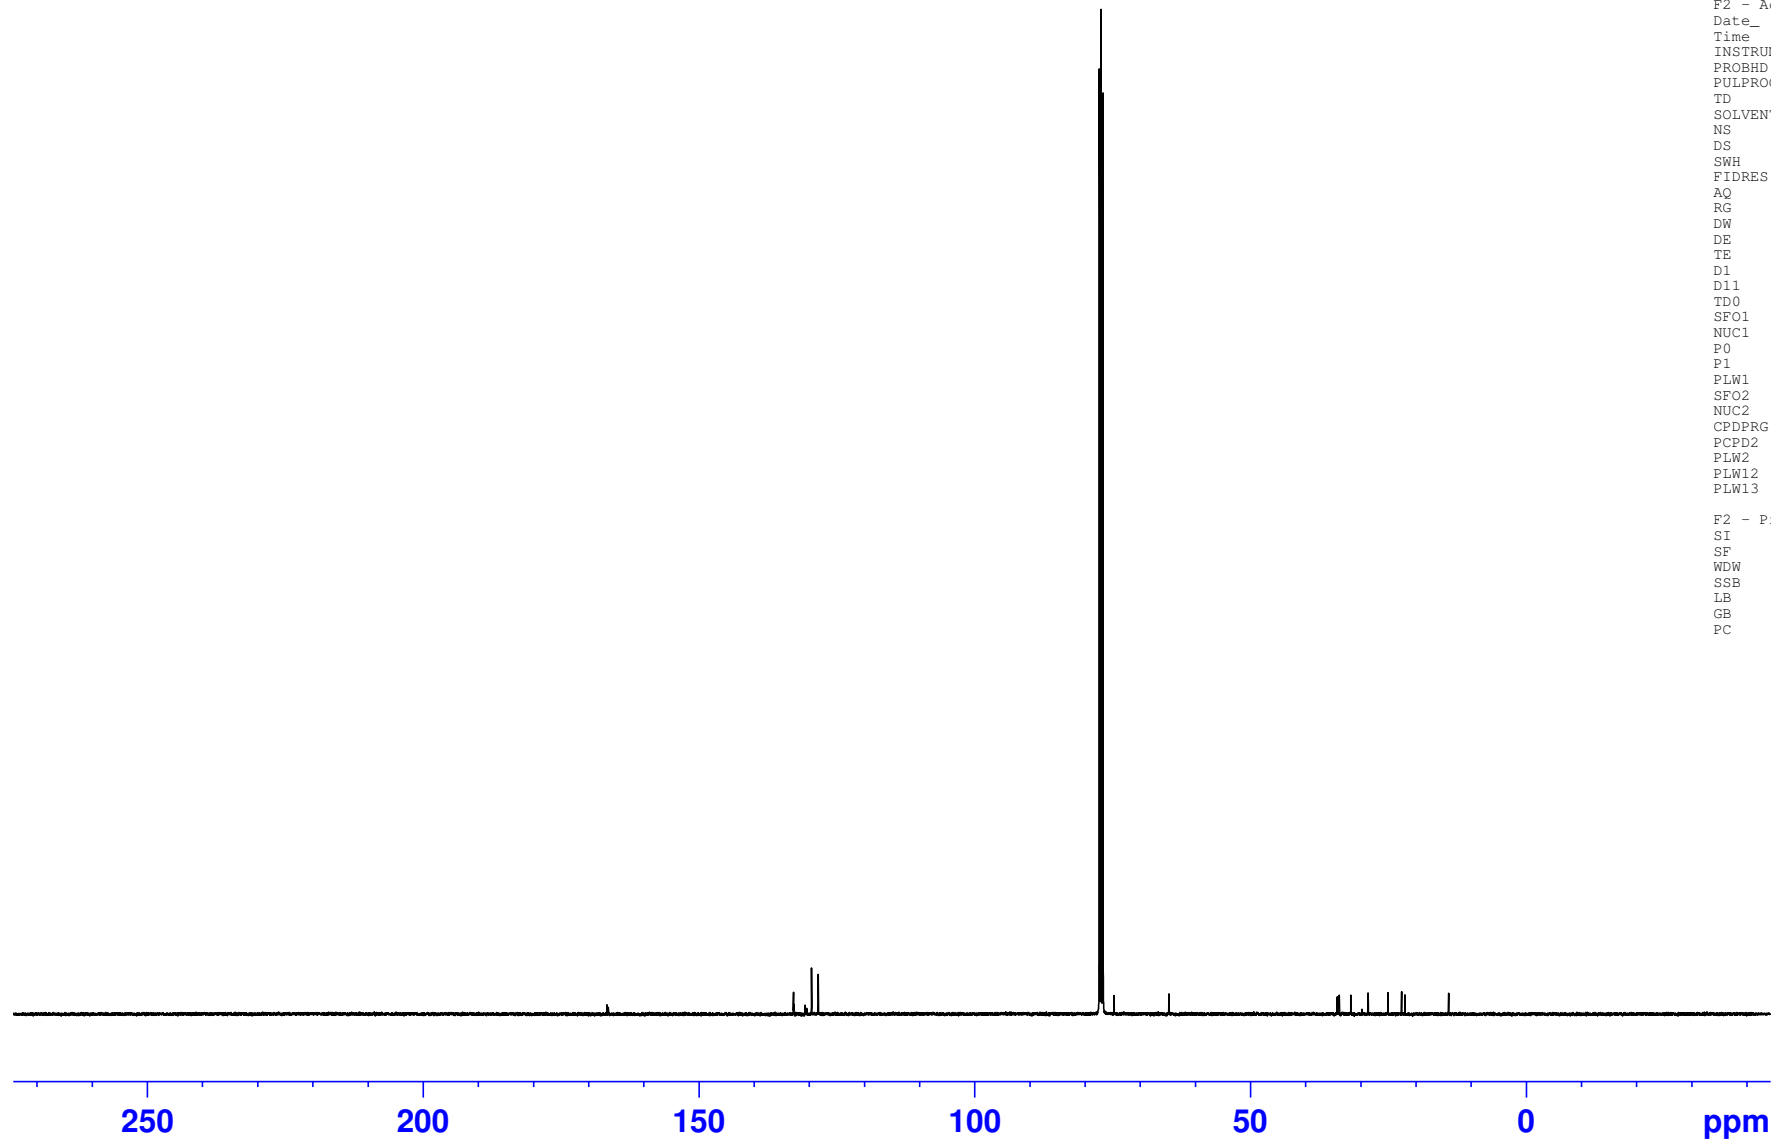

Current Data Parameters  
NAME 20190803-1819-B400\_B.11-12  
EXPNO 11  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190803  
Time 19.26 h  
INSTRUM spect  
PROBHD Z130030\_0009 (  
PULPROG zgpg30  
TD 65536  
SOLVENT CDCl3  
NS 1024  
DS 4  
SWH 32051.281 Hz  
FIDRES 0.978127 Hz  
AQ 1.0223616 sec  
RG 71.8  
DW 15.600 usec  
DE 41.97 usec  
TE 298.0 K  
D1 2.00000000 sec  
D11 0.03000000 sec  
TD0 1  
SFO1 100.6092502 MHz  
NUC1 13C  
P0 3.33 usec  
P1 10.00 usec  
PLW1 33.00000000 W  
SFO2 400.0716003 MHz  
NUC2 1H  
CPDPRG[2] waltz16  
PCPD2 90.00 usec  
PLW2 7.40000010 W  
PLW12 0.13598000 W  
PLW13 0.06839600 W

F2 - Processing parameters  
SI 32768  
SF 100.5976815 MHz  
WDW EM  
SSB 0  
LB 1.00 Hz  
GB 0  
PC 1.40