


BE219

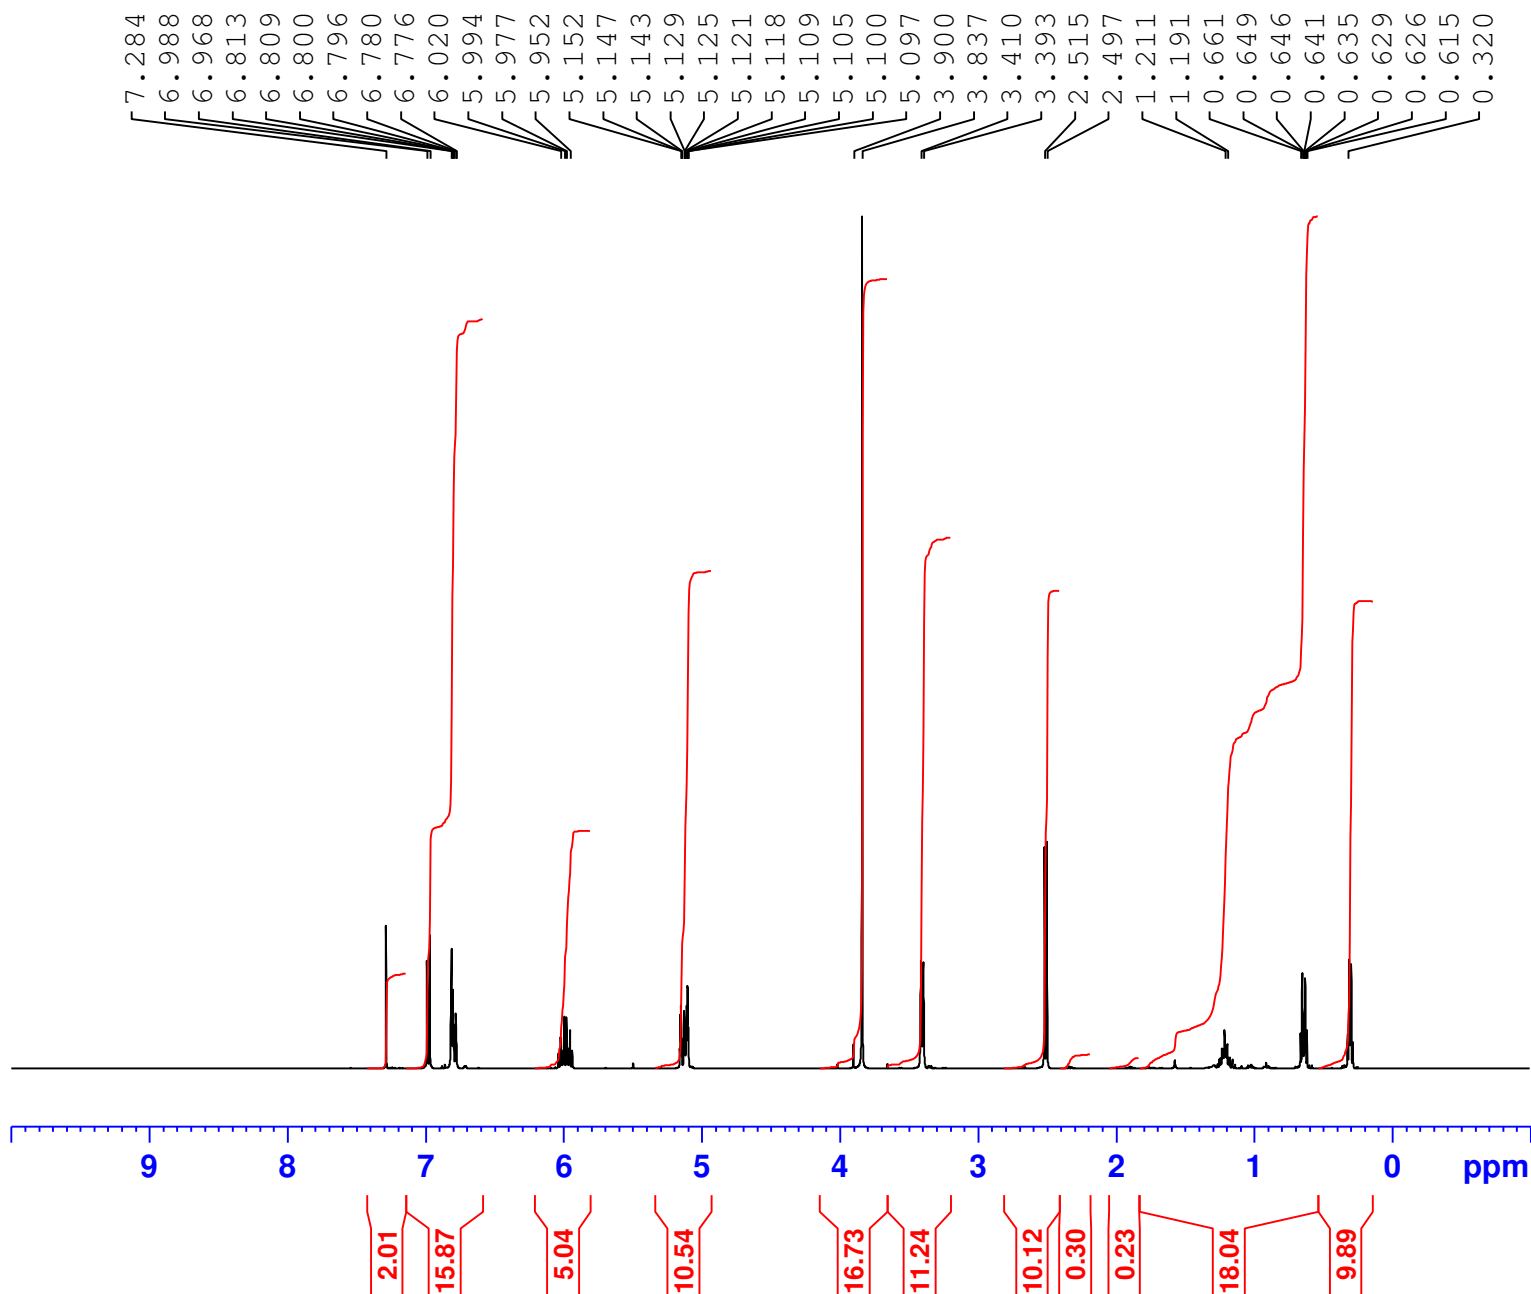

400D

Current Data Parameters
 NAME Feb27-2020
 EXPNO 490
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20200227
 Time 17.02
 INSTRUM spect
 PROBHD 5 mm PABBO BB/
 PULPROG zg30
 TD 32768
 SOLVENT CDC13
 NS 16
 DS 4
 SWH 8012.820 Hz
 FIDRES 0.244532 Hz
 AQ 2.0447233 sec
 RG 82.7
 DW 62.400 usec
 DE 6.50 usec
 TE 297.0 K
 D1 1.00000000 sec
 TD0 1

===== CHANNEL f1 =====
 SFO1 400.0524003 MHz
 NUC1 1H
 P1 9.75 usec
 PLW1 17.00000000 W

F2 - Processing parameters
 SI 32768
 SF 400.0500000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00