

HP3101

7.284  
6.965  
6.945  
6.803  
6.795  
6.775  
6.770  
5.992  
5.975  
5.151  
5.147  
5.124  
5.120  
5.108  
5.104  
5.099  
— 3.829  
3.407  
3.390  
2.605  
2.587  
2.568  
1.800  
1.781  
1.762  
1.446  
1.426  
1.329  
1.288  
0.924  
0.908  
0.891


**400D**

Current Data Parameters  
NAME Mar13-2020  
EXPNO 660  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20200313  
Time 20.33  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 32768  
SOLVENT CDC13  
NS 16  
DS 4  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 2.0447233 sec  
RG 57.33  
DW 62.400 usec  
DE 6.50 usec  
TE 297.0 K  
D1 1.00000000 sec  
TD0 1

==== CHANNEL f1 =====  
SFO1 400.0524003 MHz  
NUC1 1H  
P1 9.75 usec  
PLW1 17.00000000 W

F2 - Processing parameters  
SI 32768  
SF 400.0500000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

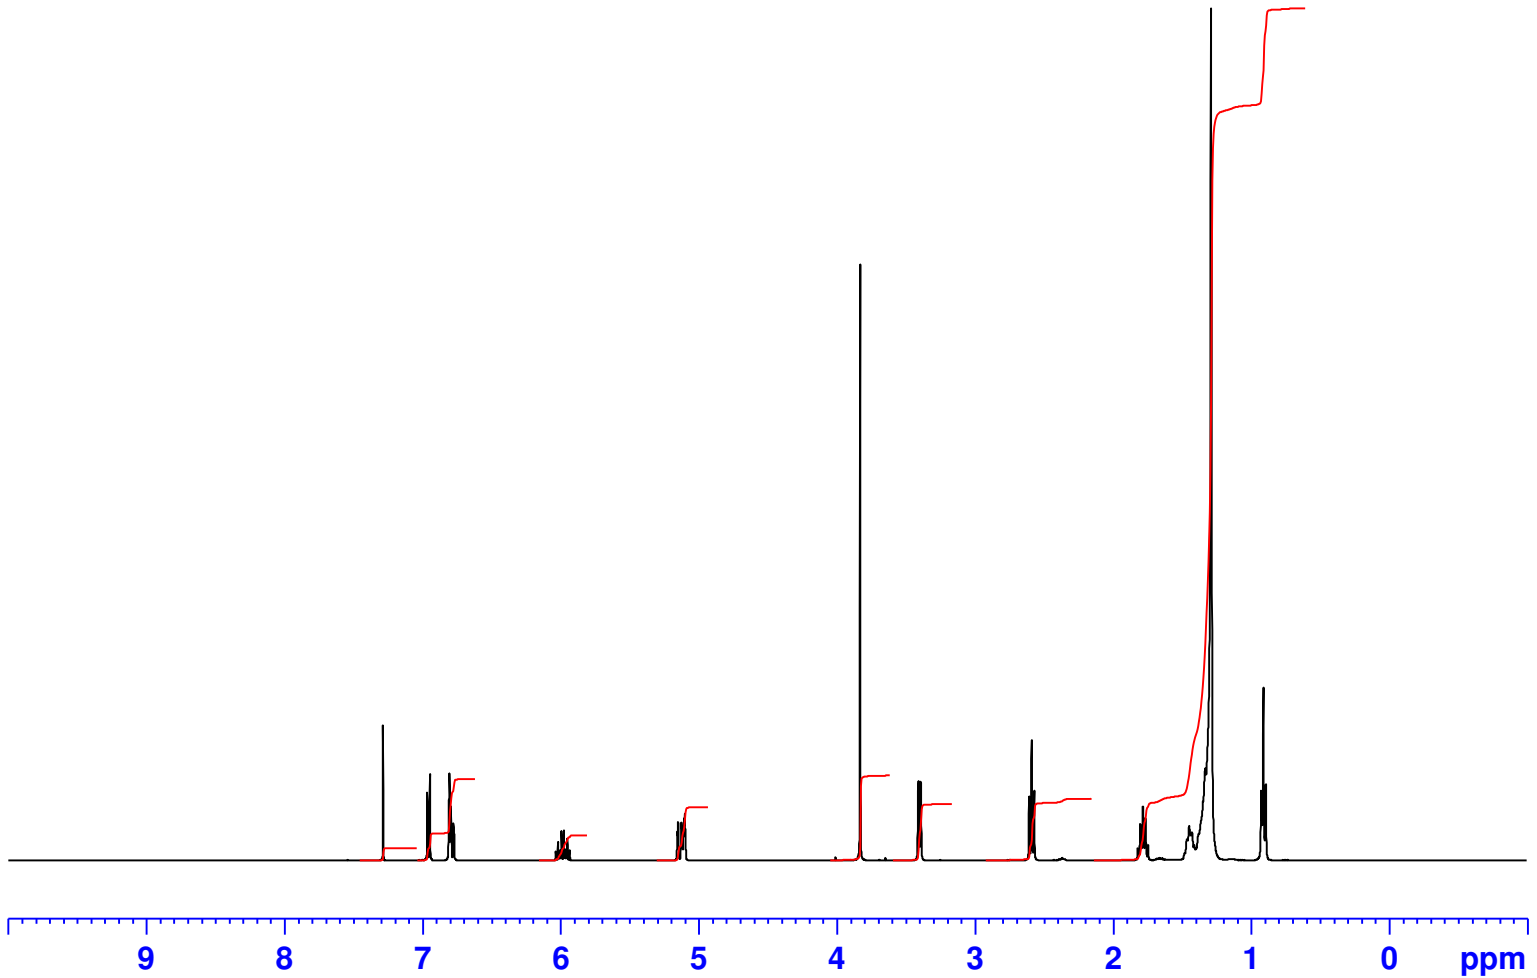

1.01  
6.63  
2.04  
4.35  
6.95  
4.63  
5.05  
69.35