


MAT002

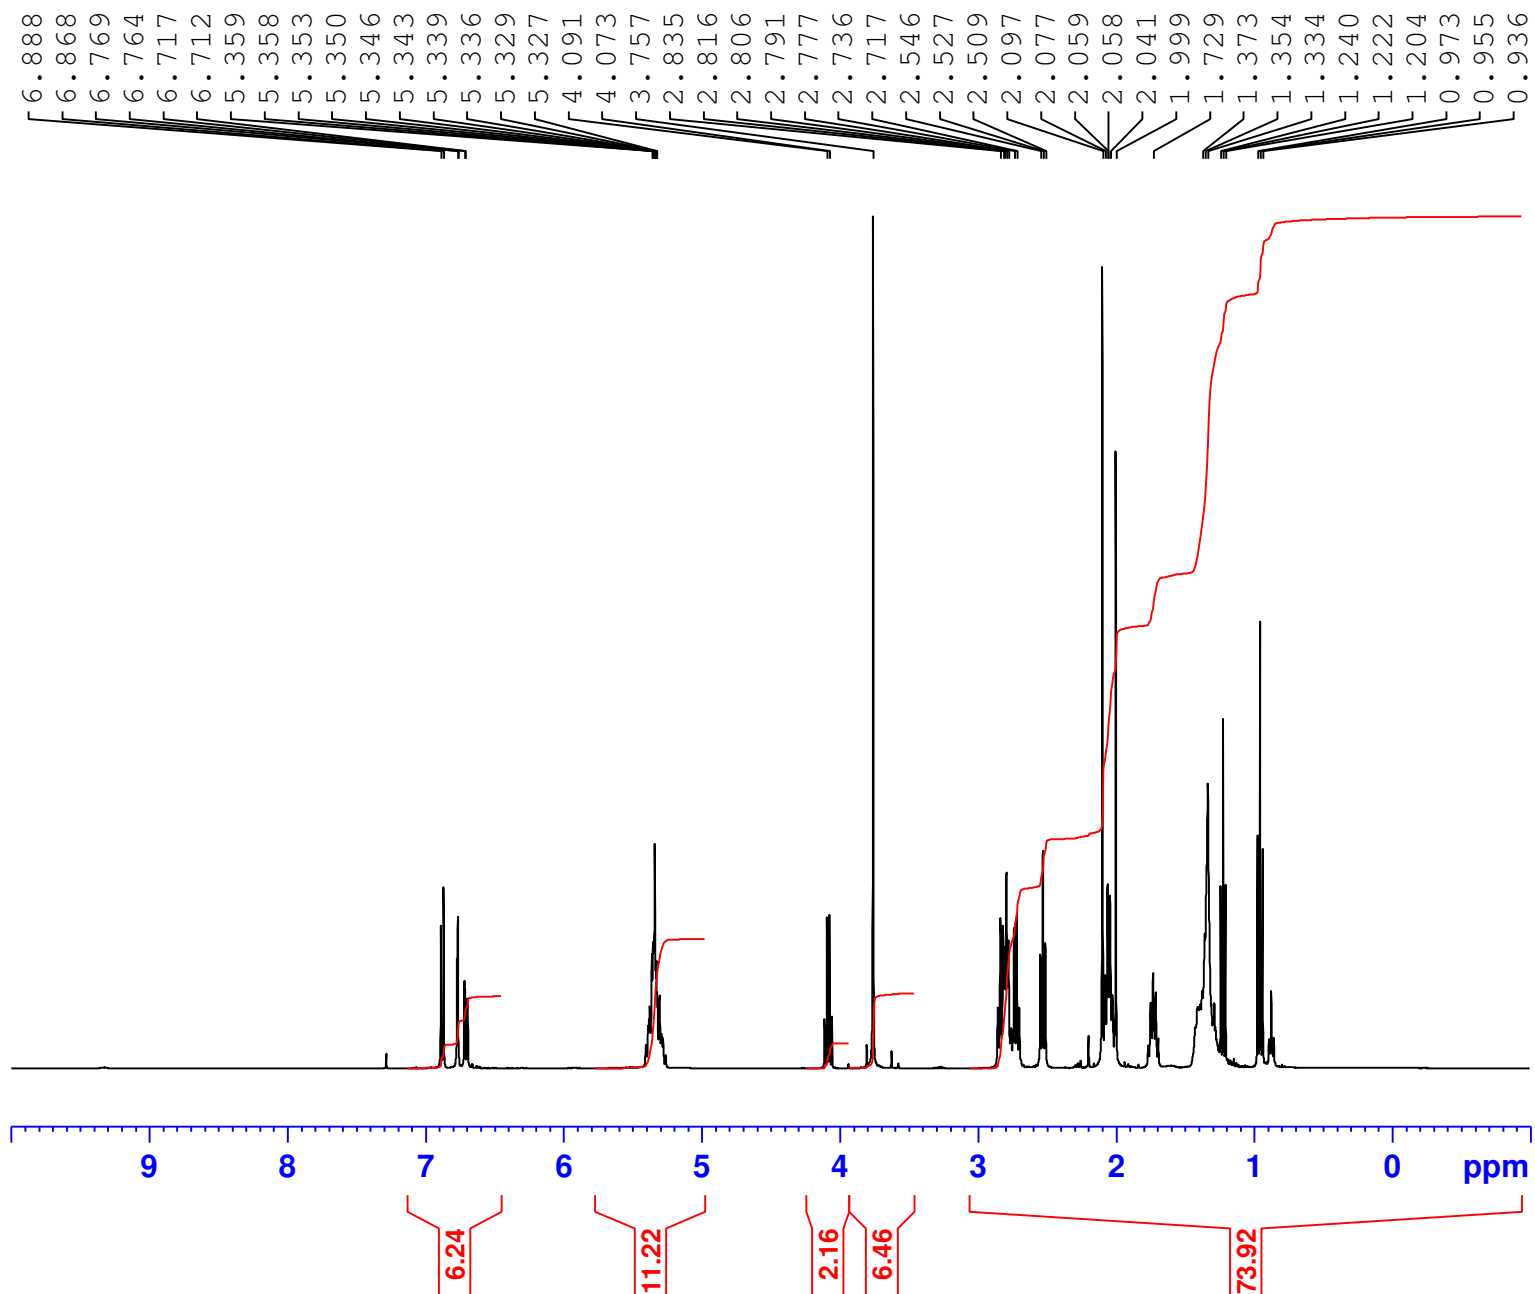

400D

Current Data Parameters
NAME Mar13-2020
EXPNO 670
PROCNO 1

F2 - Acquisition Parameters
Date_ 20200313
Time 20.37
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 32768
SOLVENT CDCl3
NS 16
DS 4
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 2.0447233 sec
RG 4.92
DW 62.400 usec
DE 6.50 usec
TE 297.0 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 400.0524003 MHz
NUC1 1H
P1 9.75 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.0500000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00