


AW:SA:SA-148-1-4

# A4

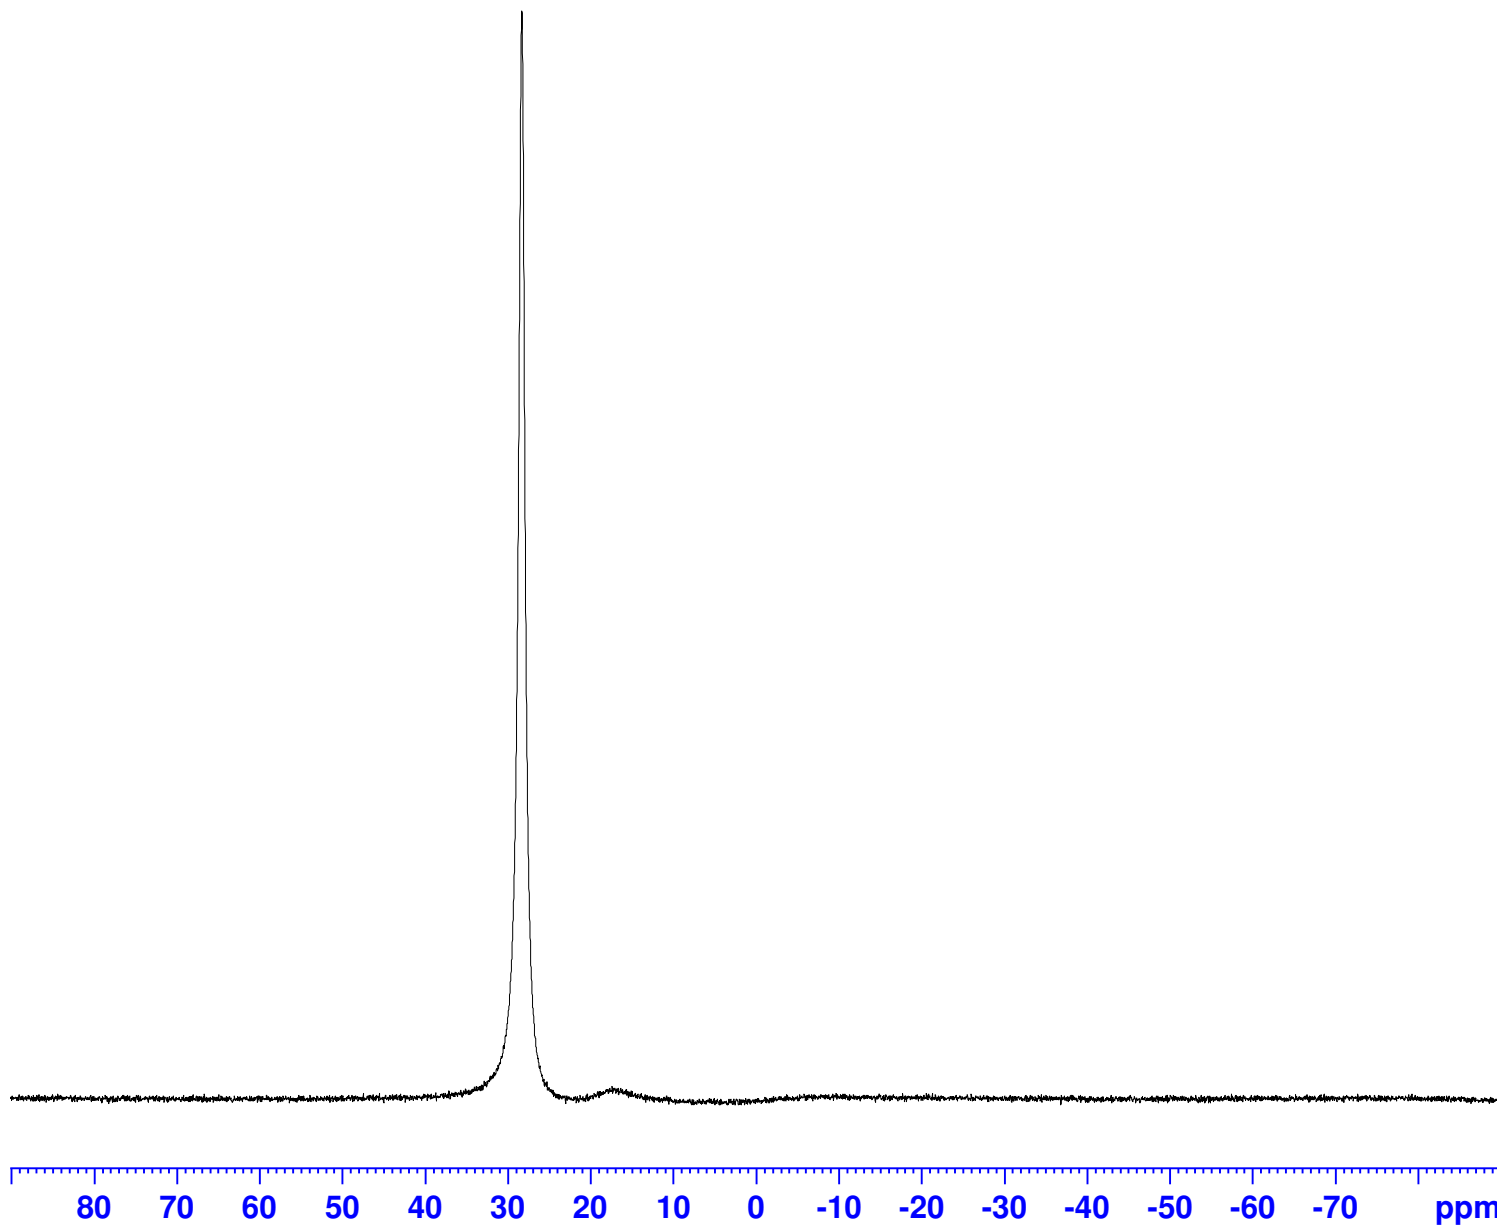

Current Data Parameters  
NAME 18153453  
EXPNO 11  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20160518  
Time 15.41  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgbs  
TD 4096  
SOLVENT CDC13  
NS 256  
DS 4  
SWH 23148.148 Hz  
FIDRES 5.651403 Hz  
AQ 0.0884736 sec  
RG 197.36  
DW 21.600 usec  
DE 6.50 usec  
TE 295.0 K  
D1 0.10000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 128.3776050 MHz  
NUC1 11B  
P1 11.88 usec  
P2 23.76 usec  
PLW1 27.22699928 W

F2 - Processing parameters  
SI 16384  
SF 128.3776050 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00