


A4

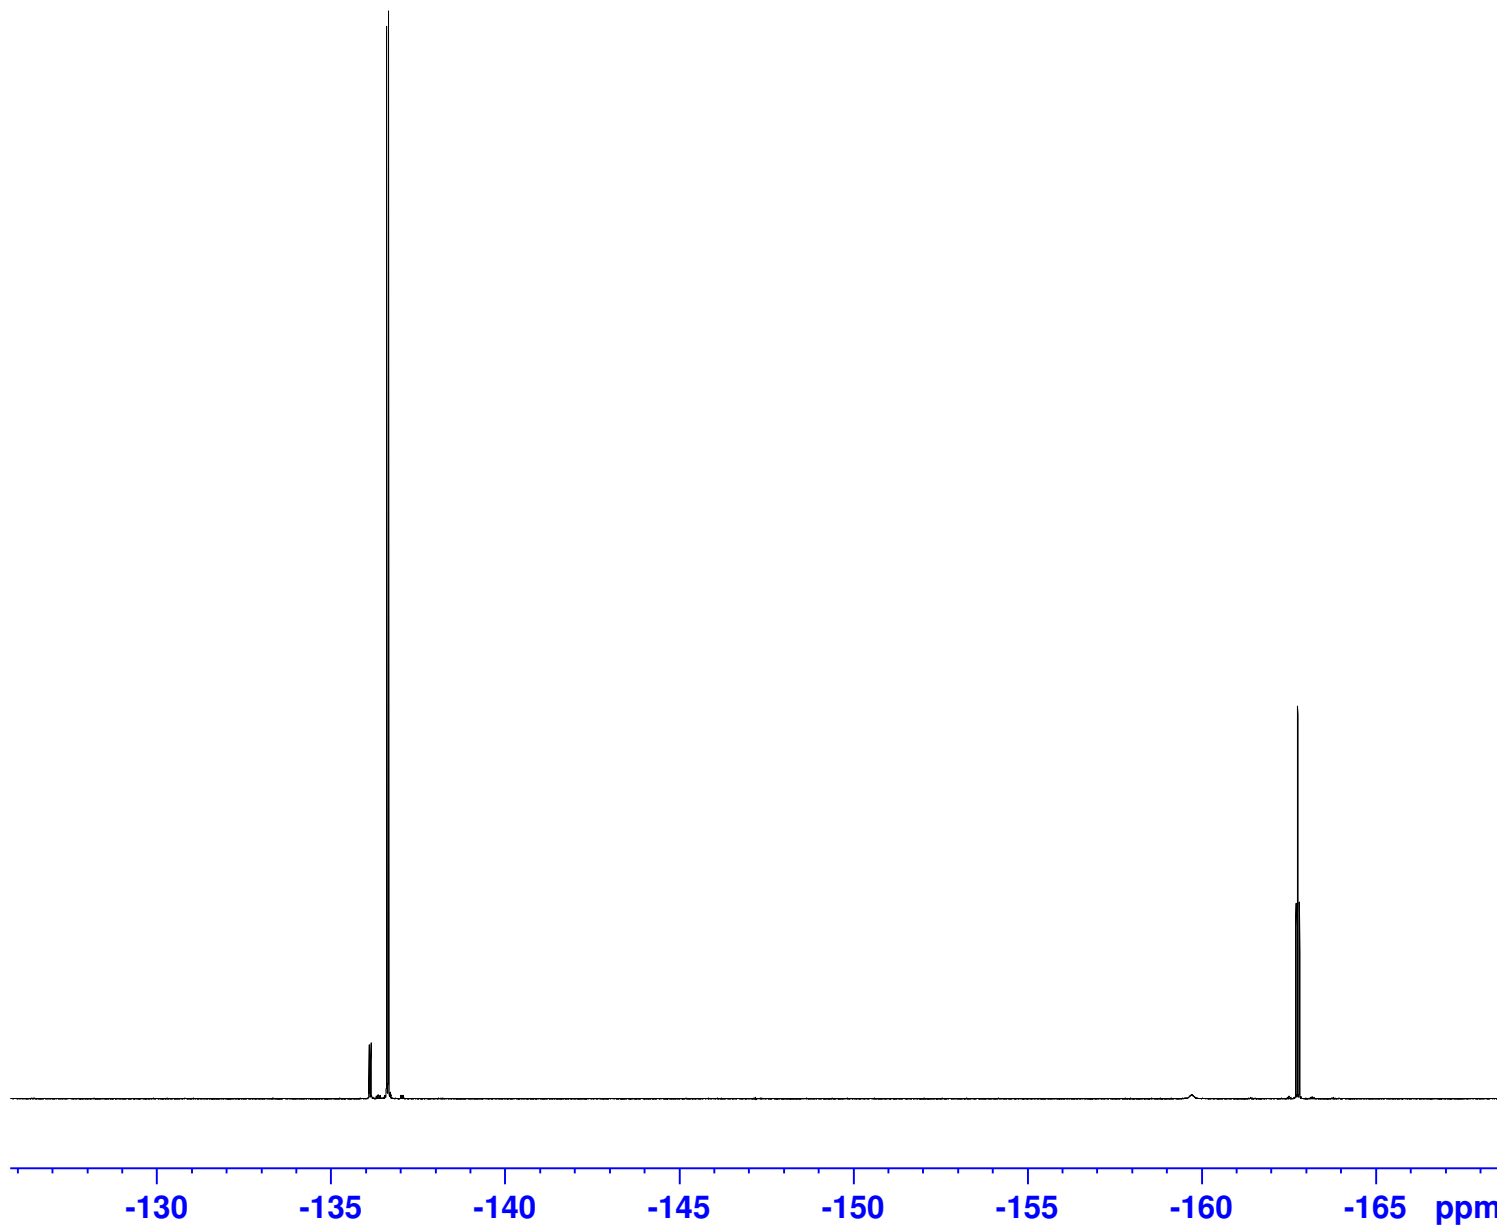

Current Data Parameters
NAME 18153453
EXPNO 14
PROCNO 1

F2 - Acquisition Parameters
Date_ 20160518
Time 15.45
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zgfhigqn180.b
TD 57216
SOLVENT CDCl3
NS 16
DS 4
SWH 16129.032 Hz
FIDRES 0.281897 Hz
AQ 1.7736959 sec
RG 197.36
DW 31.000 usec
DE 23.20 usec
TE 295.7 K
D1 1.00000000 sec
D11 0.03000000 sec
D12 0.00001000 sec
L0 1
TD0 1

===== CHANNEL f1 =====
SFO1 376.4429418 MHz
NUC1 19F
P1 12.00 usec
P26 3000.00 usec
PLW0 0 W
PLW1 28.00000000 W
SPNAM[8] Crp180,3,20.2
SPOAL8 0
SPOFFS8 0 Hz
SPW8 3.08019996 W

===== CHANNEL f2 =====
SFO2 400.1324710 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 90.00 usec
PLW2 27.20000076 W
PLW12 0.36320001 W

F2 - Processing parameters
SI 262144
SF 376.4983660 MHz
WDW EM
SSB 0
LB 0.20 Hz
GB 0
PC 2.00