

SA002

7.284
6.989
6.969
6.815
6.810
6.801
6.796
6.781
6.777
6.021
5.995
5.978
5.953
5.153
5.148
5.144
5.130
5.126
5.122
5.119
5.110
5.106
5.101
5.098
3.837
3.411
3.394
2.516
2.498
1.212
1.192
0.662
0.650
0.647
0.642
0.636
0.630
0.627
0.616
0.321
0.309


400D

Current Data Parameters
NAME Feb27-2020
EXPNO 380
PROCNO 1

F2 - Acquisition Parameters
Date_ 20200227
Time 16.20
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 32768
SOLVENT CDC13
NS 16
DS 4
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 2.0447233 sec
RG 57.33
DW 62.400 usec
DE 6.50 usec
TE 297.0 K
D1 1.00000000 sec
TD0 1

==== CHANNEL f1 =====
SFO1 400.0524003 MHz
NUC1 1H
P1 9.75 usec
PLW1 17.00000000 W

F2 - Processing parameters
SI 32768
SF 400.0500000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

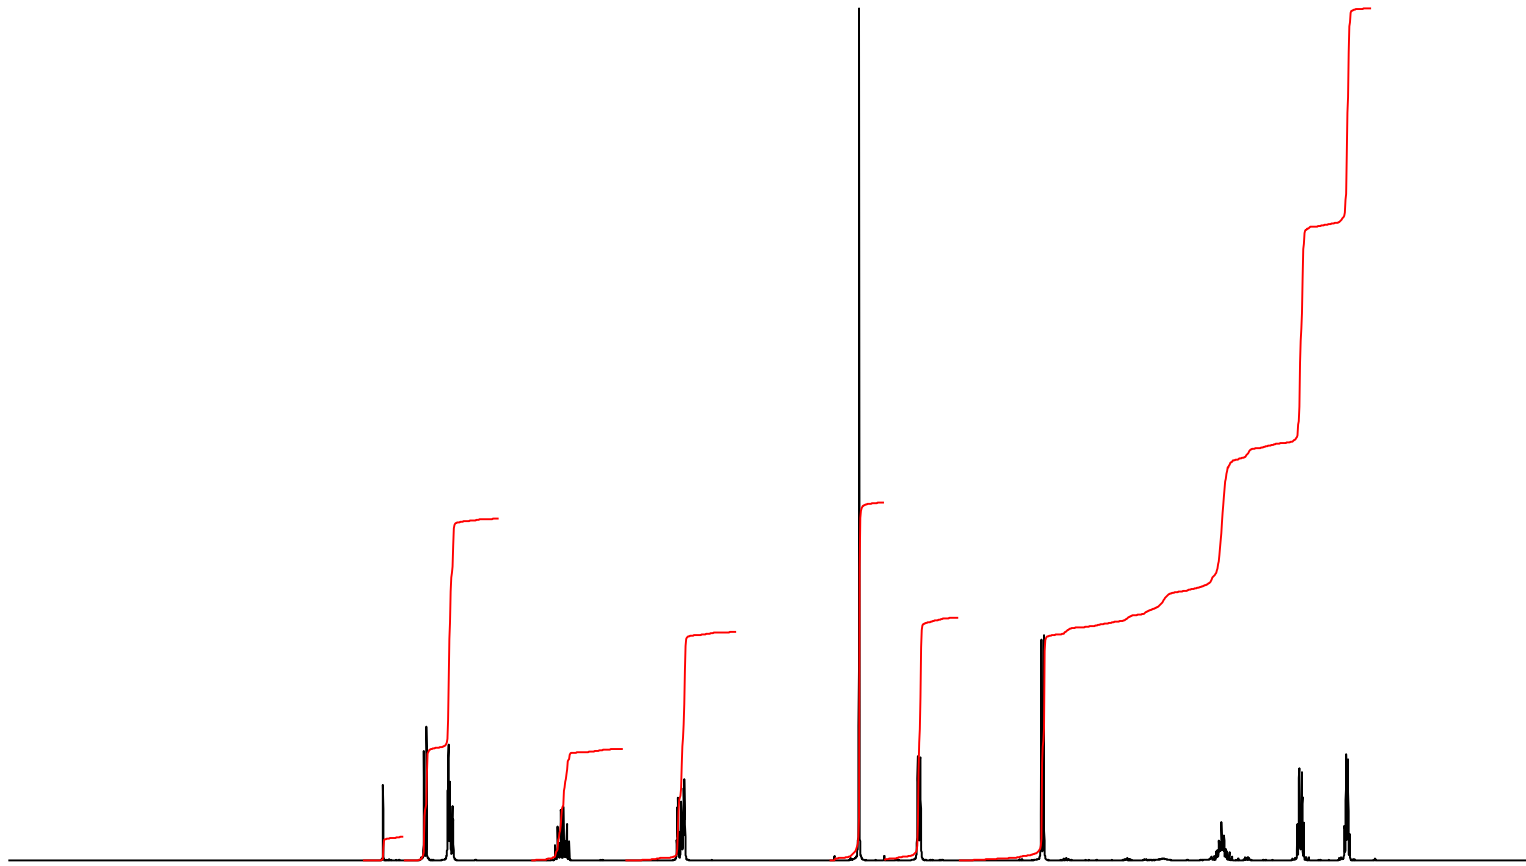

9 8 7 6 5 4 3 2 1 0 ppm

1.09
15.83
5.17
10.59
16.60
11.24
39.47