

7.345  
7.342  
7.338  
7.325  
7.322  
7.322  
7.483  
7.483  
7.208  
7.204  
7.204  
7.188  
7.185  
7.169  
7.165  
7.006  
7.003  
6.987  
6.984  
6.949  
6.929  
2.815  
2.806  
2.800  
2.791  
2.757  
2.754  
2.749  
2.746  
2.451  
2.446  
2.442  
2.435  
2.432  
2.426  
1.904  
1.886  
1.830  
1.813  
1.787  
1.776  
1.766  
1.586  
1.047  
1.021  
0.935  
0.896  
0.870  
0.020


**Av-400C**

Current Data Parameters  
NAME Aug12-2019  
EXPNO 150  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20190812  
Time 19.03  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zg30  
TD 32768  
SOLVENT CDCl3  
NS 16  
DS 2  
SWH 8012.820 Hz  
FIDRES 0.244532 Hz  
AQ 2.0447233 sec  
RG 88.22  
DW 62.400 usec  
DE 6.50 usec  
TE 294.2 K  
D1 1.00000000 sec  
TD0 1

===== CHANNEL f1 =====  
SFO1 400.2024012 MHz  
NUC1 1H  
P1 11.25 usec  
PLW1 19.95299911 W

F2 - Processing parameters  
SI 16384  
SF 400.2000000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

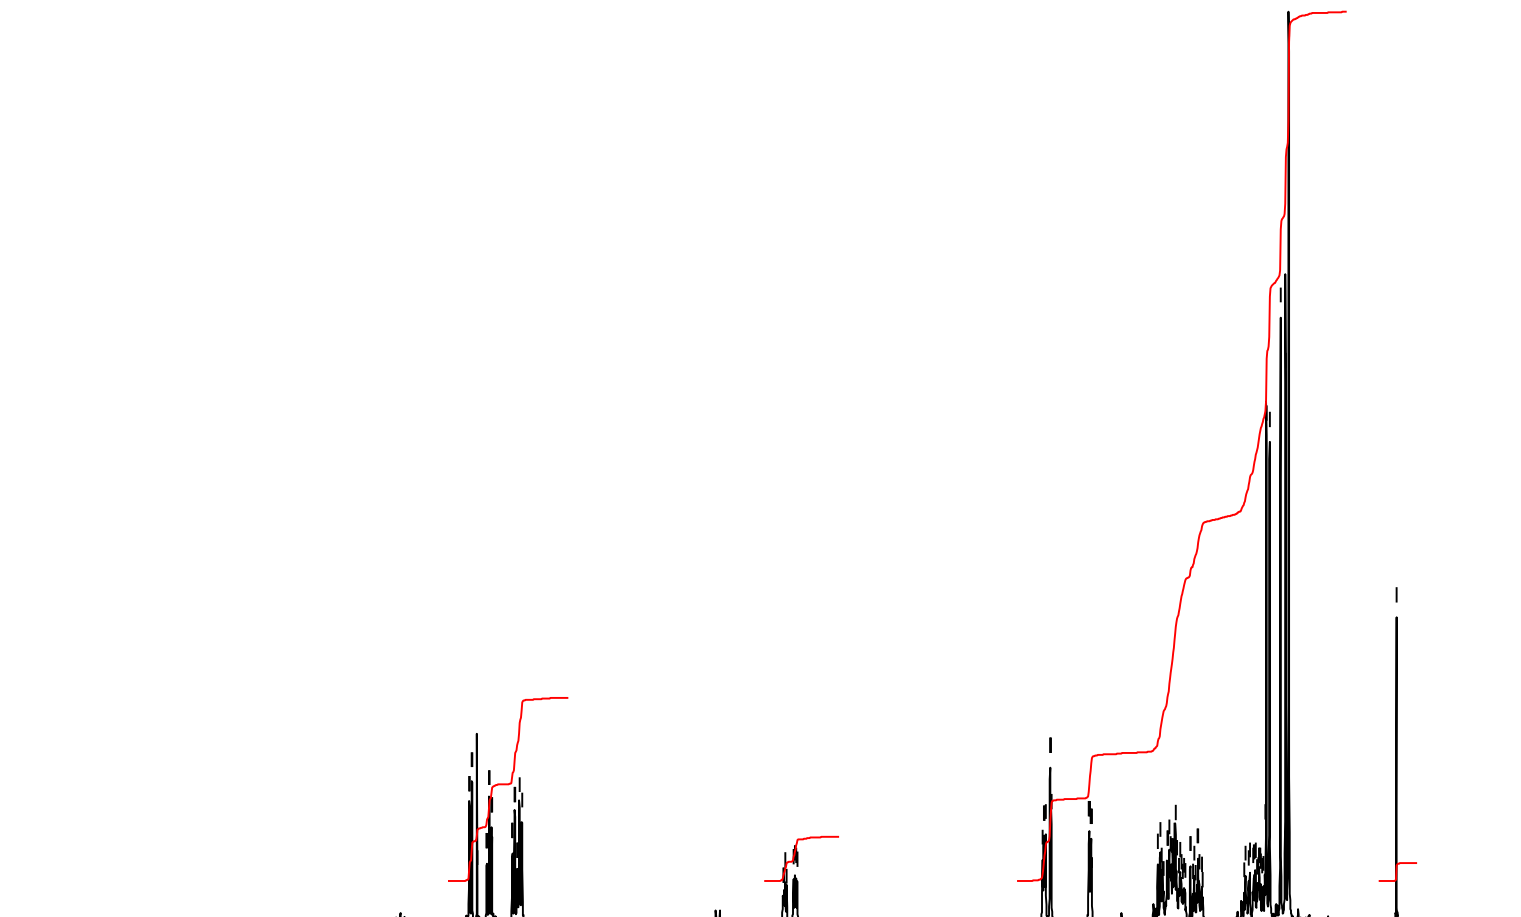

10 9 8 7 6 5 4 3 2 1 0 ppm

16.44

3.97

77.96

1.62