


AW:SA:SA-Mes-check

A4

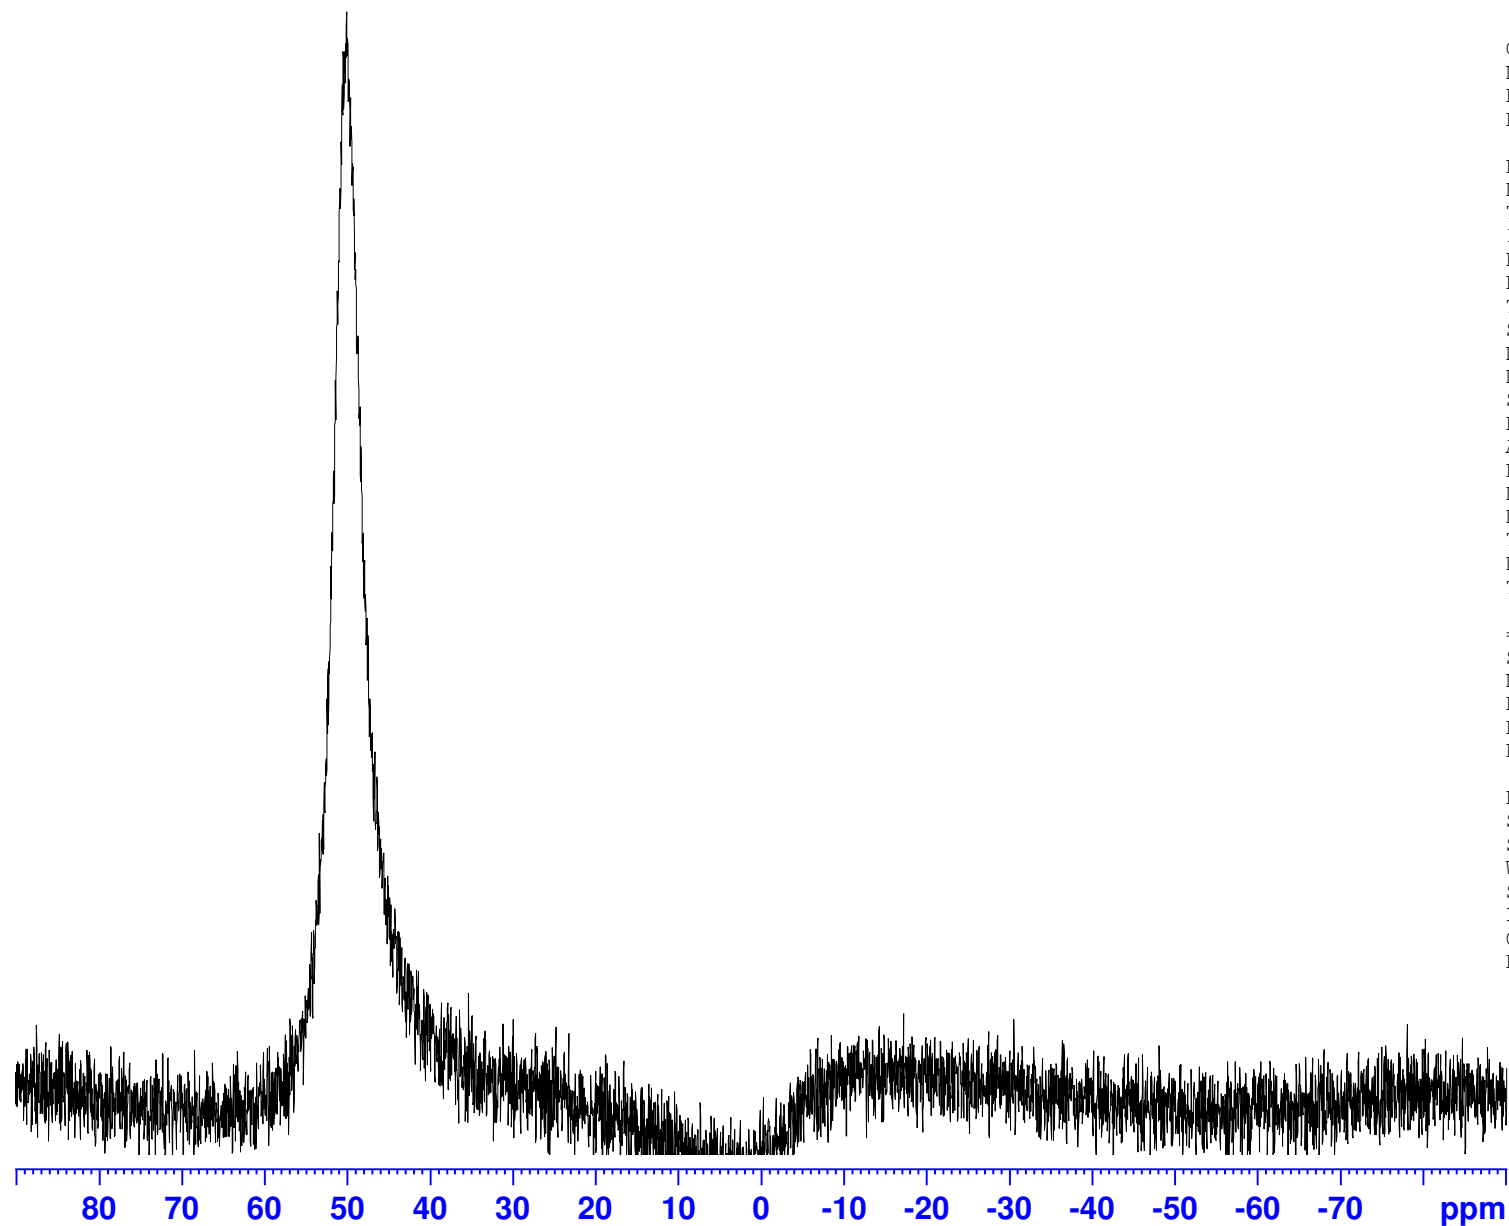

Current Data Parameters
NAME 21150237
EXPNO 11
PROCNO 1

F2 - Acquisition Parameters
Date_ 20141121
Time 15.45
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zgbs
TD 4096
SOLVENT CDC13
NS 256
DS 4
SWH 23148.148 Hz
FIDRES 5.651403 Hz
AQ 0.0884736 sec
RG 197.36
DW 21.600 usec
DE 6.50 usec
TE 296.9 K
D1 0.10000000 sec
TD0 1

===== CHANNEL f1 =====
SFO1 128.3776050 MHz
NUC1 11B
P1 11.88 usec
P2 23.76 usec
PLW1 27.22699928 W

F2 - Processing parameters
SI 16384
SF 128.3776050 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00