


# B4

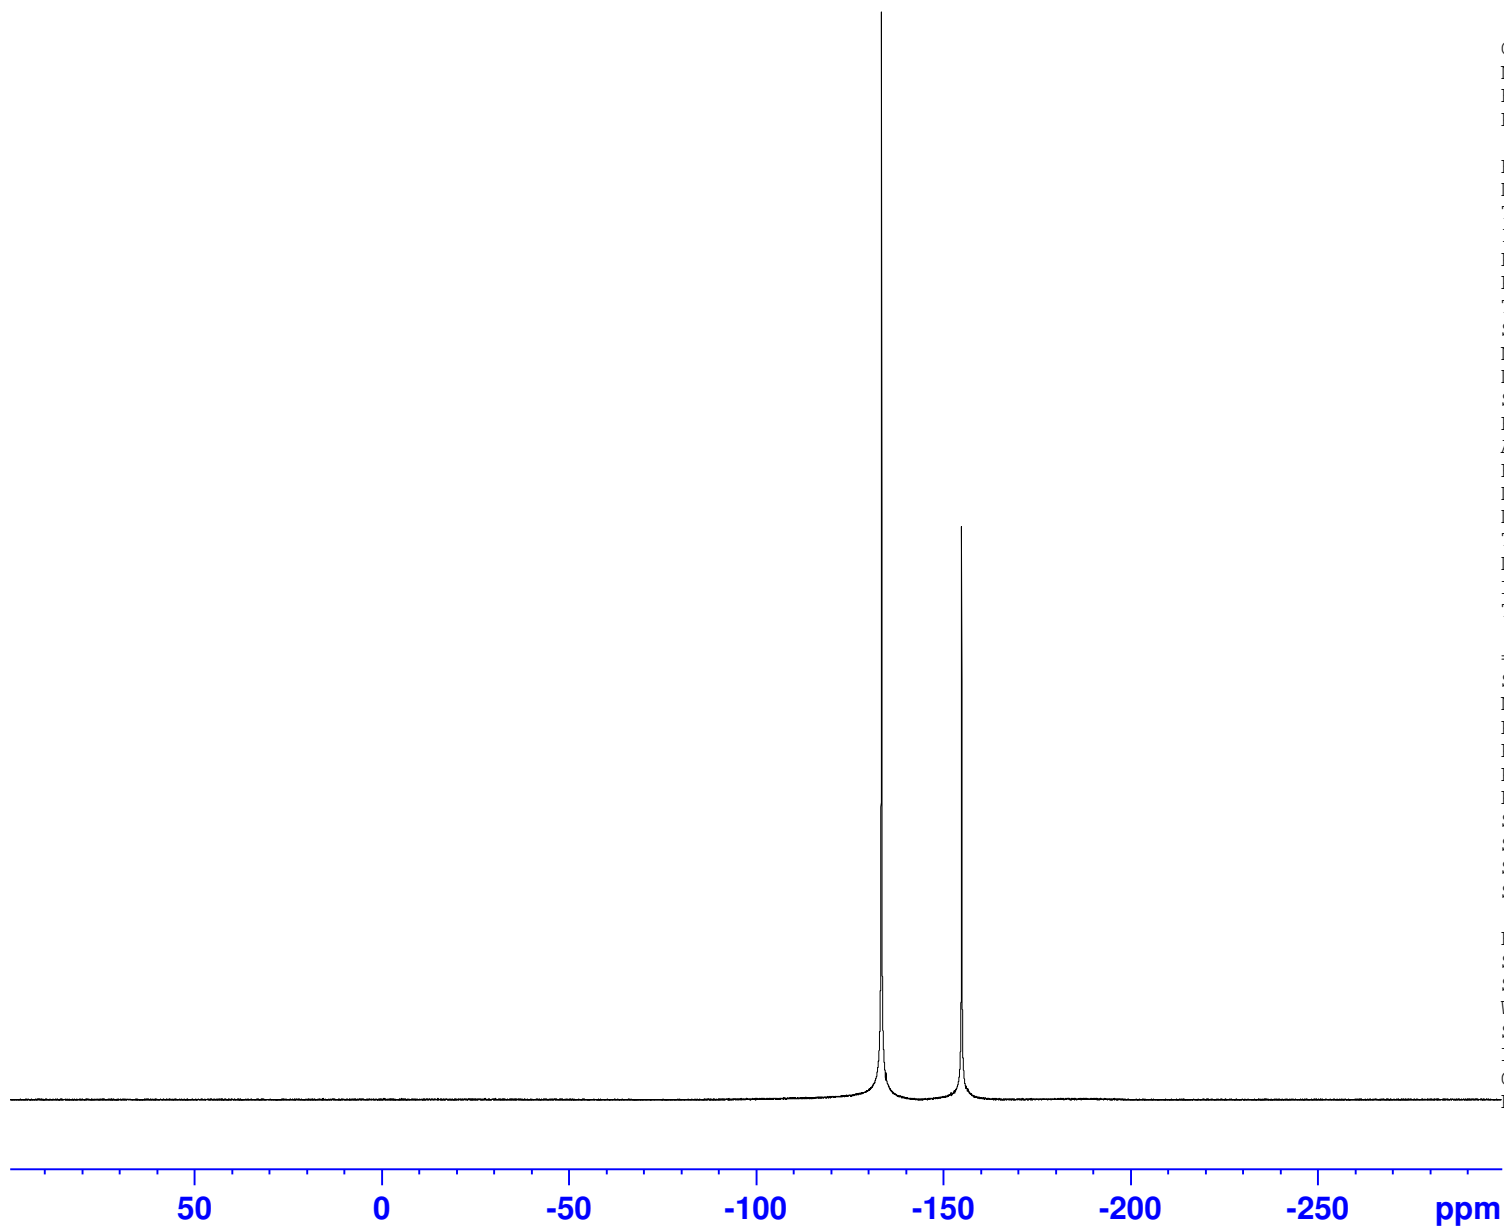

Current Data Parameters  
NAME 29191402  
EXPNO 12  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20140530  
Time 0.22  
INSTRUM spect  
PROBHD 5 mm PABBO BB/  
PULPROG zgflqn180.b  
TD 262144  
SOLVENT CDCl3  
NS 8  
DS 0  
SWH 150000.000 Hz  
FIDRES 0.572205 Hz  
AQ 0.8738133 sec  
RG 207.78  
DW 3.333 usec  
DE 20.25 usec  
TE 296.5 K  
D1 1.00000000 sec  
L0 1  
TD0 1

===== CHANNEL f1 =====  
SFO1 376.3976795 MHz  
NUC1 19F  
P1 14.00 usec  
P26 3000.00 usec  
PLW0 0 W  
PLW1 20.00000000 W  
SPNAM[8] Crp180,3,20.2  
SPOAL8 0  
SPOFFS8 0 Hz  
SPW8 2.99469995 W

F2 - Processing parameters  
SI 262144  
SF 376.4353230 MHz  
WDW EM  
SSB 0  
LB 5.00 Hz  
GB 0  
PC 2.00